



Water Analysis



- HD 2105.1 - HD 2105.2 - HD 2305.0 Portable pH meters	pag. 338
- HD 2156.1 - HD 2156.2 Portable pH and conductivity meters	pag. 342
- HD 9609 Portable pH Simulator	pag. 345
- DO 9403T-RI - DO9785T - DO 9765T pH - Redox transmitters	pag. 346
- HD 2106.1 - HD 2106.2 - HD 2306.0 Portable conductivity meters	pag. 352
- HD 2156.1 - HD 2156.2 Portable conductivity and pH meters	pag. 357
- DO 9786T - DO 9766T Conductivity transmitters	pag. 360
- HD 2109.1 - HD 2109.2 Dissolved oxygen meters	pag. 364
- HD 98569 Multi-Parameter meter: pH, conductivity, dissolved oxygen	pag. 366
- HD 3405.2- HD 2205.2 Bench-top pH meters	pag. 371
- HD 3456.2 - HD 2256.2 Bench-top pH and conductivity meters	pag. 376
- HD 3406.2 - HD 2206.2 Bench-top conductivity meters	pag. 382
- HD 3456.2 - HD 2256.2 Bench-top conductivity and pH meters	pag. 387
- HD 3409.2 Dissolved oxygen bench-top meter	pag. 393
- HD 2259.2 Dissolved oxygen and pH bench-top meter	pag. 395
- HD 22569.2 pH electrodes, conductivity probes, dissolved oxygen probes	pag. 398
- pH electrodes, conductivity probes, O ₂ probes	pag. 401
- HD 22.2 - HD 22.3 Electrode holder	pag. 404
- HD 40.1 - HD 40.2 Thermal printers	pag. 405
- HD 25.2 Bench-top turbidity meter	pag. 406

The qualitative level of our instruments is the result of a continuous evolving of the product itself. This way bring to slight differences between what reported on this manual and the instruments you bought. We can not completely exclude the presence of errors for which we apologise. Data, images and descriptions included in this catalogue can not be enforced legally. We reserve the right to perform any modification and correction at any time without notice.



HD 2105.1, HD 2105.2 TEMPERATURE-pH METERS

The **HD2105.1** and **HD2105.2** are portable instruments with a large LCD display. They measure the pH and the redox potential (ORP) in mV. They measure the temperature using Pt100 or Pt1000 immersion, penetration or contact probes.

The electrode calibration can be carried out on one, two or three points and the calibration sequence can be chosen from a list of 13 buffers.

The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

The HD2105.2 is a **datalogger**. It stored up to 34,000 pH and temperature samples which can be transferred to a PC from the instrument connected via the multi-standard RS232C serial port and USB 2.0. The storing interval, printing, and baud rate can be configured using the menu.

The HD2105.1 and HD2105.2 models are fitted with an RS232C serial port and can transfer the acquired measurements in real time to a PC or to a portable printer.

The **Max**, **Min** and **Avg** function calculate the maximum, minimum or average values.

Other functions include: the relative measurement REL, the Auto-HOLD function, and the automatic turning off that can also be excluded.

The instruments have IP67 protection degree.

INSTRUMENT TECHNICAL CHARACTERISTICS

Instrument

Dimensions	185x90x40mm
(Length x Width x Height)	470g (complete with batteries)
Weight	ABS, rubber
Materials	2x4½ digits plus symbols
Display	Visible area: 52x42mm

Operating conditions

Operating temperature	-5...50°C
Storage temperature	-25...65°C
Working relative humidity	0...90%RH without condensation
Protection degree	IP67

Power

Batteries	4 1.5V type AA batteries
Autonomy	200 hours with 1800mAh alkaline batteries
Power absorbed with instrument off	20µA
Mains	Output mains adapter 12Vdc / 1000mA

Security of memorized data

Unlimited, independent of battery charge conditions

Time

Date and time	Schedule in real time
Accuracy	1min/month max drift

Measured values storage - model **HD2105.2**

Type	2000 pages containing 17 samples each
Quantity	Total of 34000 samples
Storage interval	1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1h.

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Selectable print interval	1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1h.

USB interface - model **HD2105.2**

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Connections

Input module for the temperature probes	8-pole male DIN45326 connector
pH/mV input	Female BNC
Serial interface and USB	8-pole MiniDin connector
Mains adapter	2-pole connector (positive at centre)

Measurement of pH by Instrument

Measurement range	-2.000...+19.999pH
Resolution	0.01 or 0.001pH selectable from menu
Accuracy	±0.001pH
Input impedance	>10 ¹² Ω
Calibration error @25°C	10offset>20mV Slope<50mV/pH or Slope>63mV/pH Sensitivity < 85% or Sensitivity > 106.5%
Temperature compensation	-50...+150°C

automatic/manual



HD2110CSNM



HD2101/USB

Measurement of mV by Instrument

Measurement range	-1999.9...+1,999.9mV
Resolution	0.1mV
Accuracy	±0.1mV
Drift after 1 year	0.5mV/year

Measurement of temperature by Instrument

Pt100 measurement range	-200...+650°C
Pt1000 measurement range	-200...+650°C
Resolution	0.1°C
Accuracy	±0.1°C
Drift after 1 year	0.1°C/year

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT Temperature probes Pt100 sensor using SICRAM module

Model	Type	Application range	Accuracy
TP87	Immersion	-50°C...+200°C	±0.25°C (-50°C...+200°C)
TP4721.0	Immersion	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP473P.0	Penetration	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP474C.0	Contact	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP475A.0	Air	-50°C...+250°C	±0.3°C (-50°C...+250°C)
TP4721.5	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP4721.10	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)

Temperature drift @ 20°C 0.003%/°C

4 wire Pt100 and 2 wire Pt1000 Probes

Model	Type	Application range	Accuracy
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @ 20°C 0.005%/°C

ORDER CODES

HD2105.1: The kit is composed of: instrument HD2105.1, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software. **Electrodes, temperature probe, calibration solutions, data transfer cable for PC or printer have to be ordered separately.**

HD2110CSNM: 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole MiniDin.

C.206: Cable for instruments of the series HD21...1 and .2 to connect directly to USB input of PC.

DeltaLog9: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply at 230Vac/12Vdc-1A mains voltage.

HD40.1: The kit includes: 24-column portable thermal printer, serial interface RS232, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls

BAT-40: Spare battery pack for HD40.1 printer with built-in temperature sensor.

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm diameter.

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by power supplier SWD10 (optional).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

pH Electrodes

KP 20: Gel pH combined electrode for general use, with S7 screw connector, EPOXY body.

KP 30: Gel pH combined electrode for general use, 1m cable with BNC, EPOXY body.

KP 50: Gel pH combined electrode, porous Teflon ring junction, suitable for emulsions, demineralised water, with S7 screw connector, glass body.

KP 61: 3 diaphragm liquid filled pH combined electrode for wine, milk, cream, etc., S7 screw connector, liquid reference filling, glass body.

KP 62: 1 diaphragm gel pH combined electrode for pure water, varnishes, gel filled, S7 screw connector, glass body.

KP 63: 1 liquid filled pH combined electrode for general use, varnishes, 1m cable with BNC, glass body.

KP 64: Liquid filled pH combined electrode, Teflon ring diaphragm, for wine, varnishes, emulsions, S7 screw connector, glass body.

KP 70: Pointed gel combined pH microelectrode diam. 6 x L=70 mm., with S7 screw connector, EPOXY body, glass tip, open junction.

KP 80: Pointed gel pH combined electrode, with S7 screw connector, glass body, for cream, milk, viscous material, open junction.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

Characteristics and dimensions of the probes at page 401

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 5: 5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 10: 10m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 15: 15m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CE: S7 screw connector for pH electrode.

BNC: female BNC for extension cable

ORP Electrodes

KP 90: REDOX PLATINUM liquid filled electrode with S7 screw connector, glass body.

KP 91: Gel REDOX PLATINUM electrode, 1m cable with BNC, EPOXY body

Characteristics and dimensions of the probes at page 397

pH Buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox Buffer solutions

HDR220: Redox buffer solution 220mV 0.5 l.

HDR468: Redox buffer solution 468mV 0.5 l.

Electrolyte solutions

KCL3M Ready to use solution for electrode refilling - 100 cc

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 200ml.

Temperature probes complete with SICRAM module

TP87: Pt100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD22.3



HD 2305.0 PORTABLE pHMETER

The **HD2305.0** is a portable instrument with a large LCD display. It measures the pH and the redox potential (ORP) in mV. It measures the temperature using Pt100 or Pt1000 immersion, penetration or contact probes.

The electrode calibration can be carried out on one, two or three points at 4.01pH, 6.86pH and 9.18pH.

The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

The Max, Min and Avg function calculate the maximum, minimum or average values.

Other functions include: the relative measurement REL, the Auto-HOLD function, and the automatic turning off that can also be excluded.

The instruments have IP67 protection degree.



HD8642

HD8672

HD8692

INSTRUMENT TECHNICAL CHARACTERISTICS

Measured quantities: pH, mV, °C, °F

Instrument

Dimensions (Length x Width x Height)	140x88x38mm
Weight	160g (complete with batteries)
Materials	ABS
Display	2x4½ digits plus symbols
Visible area:	52x42mm

Working conditions

Operating temperature	-5...50°C
Storage temperature	-25...65°C
Working relative humidity	0...90%RH without condensation

Protection degree

IP67

Power

Batteries	3 1.5V type AA batteries
Autonomy	200 hours with 1800mAh alkaline batteries
Power absorbed with instrument off	20µA

Connections

Input module for the temperature probes	8-pole male DIN45326 connector
pH/mV input	Female BNC

Measurement of pH by Instrument

Measurement range	-2.000...+19.999pH
Resolution	0.01
Accuracy	±0.01pH±1 digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	Offset<20mV
	Slope<50mV/pH or Slope>63mV/pH
	Sensitivity < 85% or Sensitivity > 106.5%

Measurement of mV by Instrument

Measurement range	-1999.9...+1,999.9mV
Resolution	0.1mV
Accuracy	±0.1mV
Drift after 1 year	0.5mV/year

Measurement of temperature by Instrument

Pt100 measurement range	-200...+650°C
Pt1000 measurement range	-200...+650°C
Resolution	0.1°C
Accuracy	±0.1°C
Drift after 1 year	0.1°C/year

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT

Temperature probes Pt100 sensor using SICRAM module

Model	Type	Application range	Accuracy
TP87	Immersion	-50°C...+200°C	±0.25°C (-50°C...+200°C)
TP472I.0	Immersion	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP473P.0	Penetration	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP474C.0	Contact	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP475A.0	Air	-50°C...+250°C	±0.3°C (-50°C...+250°C)
TP472I.5	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP472I.10	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)

Temperature drift @ 20°C 0.003%/°C

4 wire Pt100 and 2 wire Pt1000 Probes

Model	Type	Application range	Accuracy
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @ 20°C 0.005%/°C

ORDER CODES

HD2305.0: The kit is composed of: instrument HD2305.0, 3 1.5V alkaline batteries, operating manual, case.

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by power supplier SWD10 (optional).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

pH Electrodes

KP 20: Gel pH filled combined electrode for general use, with S7 screw connector, EPOXY body.

KP 30: Gel pH combined electrode for general use, 1m cable with BNC, EPOXY body.

KP 50: Gel pH combined electrode, porous Teflon ring junction, suitable for emulsions, demineralised water, with S7 screw connector, glass body.

KP 61: 3 diaphragm liquid filled pH combined electrode for wine, milk, cream, etc., S7 screw connector, liquid reference filling, glass body.

KP 62: 1 diaphragm gel pH combined electrode for pure water, varnishes, gel filled, S7 screw connector, glass body.

KP 63: 1 liquid filled pH combined electrode for general use, varnishes, 1m cable with BNC, glass body.

KP 64: Liquid filled pH combined electrode, Teflon ring diaphragm, for wine, varnishes, emulsions, S7 screw connector, glass body.

KP 70: Pointed gel combined pH microelectrode diam. 6 x L=70 mm., with S7 screw connector, EPOXY body, glass tip, open junction.

KP 80: Pointed gel pH combined electrode, with S7 screw connector, glass body, for cream, milk, viscous material, open junction.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

Characteristics and dimensions of the probes at page 401

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 5: 5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 10: 10m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 15: 15m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CE: S7 screw connector for pH electrode.

BNC: female BNC for extension cable

ORP Electrodes

KP 90: REDOX PLATINUM liquid filled electrode with S7 screw connector, glass body.

KP 91: Gel REDOX PLATINUM electrode, 1m cable with BNC, EPOXY body

Characteristics and dimensions of the probes at page 402

pH Buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox Buffer solutions

HDR220: Redox buffer solution 220mV 0.5 l.

HDR468: Redox buffer solution 468mV 0.5 l.

Electrolyte solutions

KCL3M Ready to use solution for electrode refilling – 100 cc

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fl uorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 200ml.

Temperature probes complete with SICRAM module

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD22.3



CP





HD 2156.1, HD 2156.2 pH METER - CONDUCTIVITY METER - THERMOMETER

The **HD2156.1** and **HD2156.2** are portable instruments with a large LCD display. They measure pH, mV, redox potential (ORP), conductivity, liquid resistivity, total dissolved solids (TDS) and salinity using combined 4-ring and 2-ring conductivity/temperature probes. Temperature only is measured by Pt100 or Pt1000 immersion, penetration or contact probes.

The pH electrode calibration, as well as manual, can be carried out on one, two or three points and the calibration sequence can be chosen from a list of 13 buffers.

The probe calibration can be performed automatically in one or more of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions.

The HD2156.2 instrument is a **logger**. It memorizes up to 20,000 sets of three measurements composed of pH or mV, conductivity or resistivity or TDS or salinity and temperature: these data can be transferred to a PC from the instrument connected via the multi-standard RS232C serial port and USB 2.0. The storing interval, printing, and baud rate can be configured using the menu.

The HD2156.1 and HD2156.2 models are fitted with an RS232C serial port and can transfer the acquired measurements to a PC or to a portable printer in real time.

The *Max*, *Min* and *Avg* function calculates the maximum, minimum or average values.

Other functions include: the Auto-HOLD function and the automatic turning off which can also be excluded.

The instruments have IP67 protection degree.

INSTRUMENT TECHNICAL CHARACTERISTICS

Measured quantities: pH, mV, χ , Ω , TDS, NaCl, °C, °F

Instrument

Dimensions (Length x Width x Height)	185x90x40mm
Weight	470g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ digits plus symbols Visible area: 52x42mm

Operating conditions

Working temperature	-5...50°C
Storage temperature	-25...65°C
Working relative humidity	0...90%RH without condensation
Protection degree	IP67

Power

Batteries	4 1.5V type AA batteries
Autonomy	200 hours with 1800mAh alkaline batteries
Power absorbed with instrument off	20µA
Mains	Output mains adapter 9Vdc / 250mA

Security of memorized data

Unlimited, independent of battery charge conditions

Time

Date and time	Schedule in real time
Accuracy	1min/month max error

Measured values storage - model **HD2156.2**

Type	2000 pages containing 10 samples each
Quantity	20,000 sets of three measurements composed of pH or mV, χ or Ω or TDS or salinity and temperature.
Storage interval	1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1h.

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Immediate print interval	1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1h.

USB interface - model **HD2156.2**

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Connections

pH/mV input	Female BNC connector
Conductivity input	8-pole male DIN45326 connector
Serial interface and USB	8-pole MiniDin connector
Mains adapter	2-pole connector (positive at centre)

Measurement of pH by Instrument

Measurement range	-2.000...+19.999pH
Resolution	0.01 or 0.001pH selectable from menu
Accuracy	±0.001pH ±1 digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	Offset > 20mV Slope > 63mV/pH or Slope < 50mV/pH Sensitivity > 106.5% or Sensitivity < 85%

Measurement of mV by Instrument

Measurement range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	±0.1mV ±1 digit
Drift after 1 year	0.5mV/year

Measurement of conductivity			Measurement of salinity		
Measuring range	0.00...19.99µS/cm	Resolution	0.01µS/cm	Measurement range	0.000...1.999g/l
Kcell=0.1					1mg/l
Measuring range	0.0...199.9µS/cm		0.1µS/cm	Measurement range	2.00...19.99g/l
Kcell=1			1µS/cm		10mg/l
	200...1999µS/cm		0.01mS/cm	Accuracy (salinity)	±0.5%1digit
	2.00...19.99mS/cm		0.1mS/cm		
Measuring range	20.0...199.9mS/cm		1mS/cm	Temperature compensation	
Kcell=10				automatic/manual	0...100°C with α_T selectable from 0.00 to 4.00%/°C
Accuracy (conductivity)	±0.5%1digit			Reference temperature	20°C or 25°C
				χ / TDS Conversion factor	0.4...0.8
				Cell constant K (cm ⁻¹)	0.1, 0.7, 1.0 and 10.0
Measurement of resistivity			Standard solutions automatically detected @25°C		
Measuring range	till 100MΩ·cm/(*)				147µS/cm
Kcell=0.1					1413µS/cm
Measuring range	5.0...199.9Ω·cm		0.1Ω·cm		12880µS/cm
Kcell=1			1Ω·cm		111800µS/cm
	1.00k...19.99kΩ·cm		0.01kΩ·cm		
	20.0k...99.9kΩ·cm		0.1kΩ·cm		
	100k...999kΩ·cm		1kΩ·cm		
	1...10MΩ·cm		1MΩ·cm		
Measuring range	0.5...5.0Ω·cm		0.1Ω·cm		
Kcell=10					
Accuracy (resistivity)	±0.5%±1digit				
Measurement of total dissolved solids (with coefficient χ/TDS=0.5)			Measurement of temperature		
Measuring range	0.00...19.99mg/l		0.05mg/l	Pt100 measuring range	-50...+200°C
Kcell=0.1				Pt1000 measuring range	-50...+200°C
Measuring range	0.0...199.9mg/l		0.5mg/l	Resolution	0.1°C
Kcell=1			1mg/l	Accuracy	±0.25°C
	200...1999mg/l		1mg/l	Drift after 1 year	0.1°C/anno
	2.00...19.99g/l		0.01g/l	Preset cell constant values:	K=0,01 - K=0,1 - K=1, K=10
	20.0...99.9g/l		0.1g/l		
Measuring range	100...999g/l		1g/l		
Kcell=10					
Accuracy (conductivity)			±0.5%1digit		

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity (µS/cm)	Resistivity (MΩ·cm)	Conductivity (µS/cm)	Resistivity (MΩ·cm)
0.001 µS/cm	1000 MΩ·cm	0.01 µS/cm	100 MΩ·cm
0.002 µS/cm	500 MΩ·cm	0.02 µS/cm	50 MΩ·cm
0.003 µS/cm	333 MΩ·cm	0.03 µS/cm	33 MΩ·cm
0.004 µS/cm	250 MΩ·cm	0.04 µS/cm	25 MΩ·cm
...

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT		
2 and 4 electrode conductivity probes		
ORDER CODE	MEASUREMENT RANGE	DIMENSIONS
SP06T	K=0.7 5µS...200mS/cm 0...90°C 4-electrode cell in POCAN/Platinum	
SPT 400.001 not suitable for HD 2306.0	K=0.01 0,05...19,9µS/cm 2-electrode cell AlSi 316 - Teflon	
SPT01G	K=0.1 0.1µS...500µS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT1G	K=1 10µS...10mS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT10G	K=10 500µS...200mS/cm 0...80°C 2-electrode cell in Glass/Platinum	

Temperature probes with connector 4 wire Pt100 and 2 wire Pt1000 sensor

Model	Type	Working range	Accuracy
TP47.100	Pt100 4 wires	-50...+200°C	Class A
TP47.1000	Pt1000 2 wires	-50...+200°C	Class A
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @20°C 0.005%/°C

ORDER CODES

HD2156.1: The kit is composed of: instrument HD2156.1, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software. **Other pH electrodes, conductivity and temperature probes must be ordered separately.**

HD2156.2K: The kit is composed of: instrument HD2156.2 datalogger, 4 1.5V alkaline batteries, operating software DeltaLog9. **Other pH electrodes, conductivity and temperature probes must be ordered separately.**

pH/mV probes, conductivity probes, temperature probes, standard calibration solutions for various types of measurements, connection cables for pH electrodes with S7 connector, cables for data transfer to PC or printer have to be ordered separately.

HD2110CSNM: 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

C.206: Serial connection cable with USB connector for PC and 8-pole MiniDin male connector for the instrument.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole MiniDin (not suitable for HD2156.1K).

DeltaLog9: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply 100-240 Vac/12Vdc-1A mains voltage

HD40.1: 24-column portable thermal printer, serial interface, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm in diameter.

BAT-40: Spare battery pack for HD40.1 printer with built-in temperature sensor.

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by bench-top meters of the series HD22...with cable HD22.2.1 (optional) or power supplier SWD10 (optional).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

pH Electrodes

KP 20: Gel pH filled combined electrode for general use, with S7 screw connector, EPOXY body.

KP 30: Gel pH combined electrode for general use, 1m cable with BNC, EPOXY body.

KP 50: Gel pH combined electrode, porous Teflon ring junction, suitable for emulsions, demineralised water, with S7 screw connector, glass body.

KP 61: 3 diaphragm liquid filled pH combined electrode for wine, milk, cream, etc., S7 screw connector, liquid reference filling, glass body.

KP 62: 1 diaphragm gel pH combined electrode for pure water, varnishes, gel filled, S7 screw connector, glass body.

KP 63: 1 liquid filled pH combined electrode for general use, varnishes, 1m cable with BNC, glass body.

KP 64: Liquid filled pH combined electrode, Teflon ring diaphragm, for wine, varnishes, emulsions, S7 screw connector, glass body.

KP 70: Pointed gel combined pH microelectrode diam. 6 x L=70 mm., with S7 screw connector, EPOXY body, glass tip, open junction.

KP 80: Pointed gel pH combined electrode, with S7 screw connector, glass body, for cream, milk, viscous material, open junction.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

Characteristics and dimensions of the probes at page 401

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 5: 5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 10: 10m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 15: 15m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CE: S7 screw connector for pH electrode.

BNC: female BNC for extension cable

ORP Electrodes

KP 90: REDOX PLATINUM liquid filled electrode with S7 screw connector, glass body.

KP 91: Gel REDOX PLATINUM electrode, 1m cable with BNC, EPOXY body

Characteristics and dimensions of the probes at page 402

pH Buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox Buffer solutions

HDR220: Redox buffer solution 220mV 0.5 l.

HDR468: Redox buffer solution 468mV 0.5 l.

Electrolyte solutions

KCL3M Ready to use solution for electrode refilling - 100 cc

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fl uorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 200ml.

Temperature probes complete with SICRAM module

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.





TECHNICAL CHARACTERISTICS

pH simulation:	0 ÷ 14 pH
pH resolution:	0.1 pH
pH accuracy 20 ÷ 25°C:	0.002 pH
Thermal drift:	±0.0005 pH/°C from -5°C to 20°C and from 25°C to 50°
mV simulation:	±1999 mV
mV resolution:	1 mV
mV accuracy:	±100 µV
Thermal drift mV scale:	-199.9 ... +199.9: ±0.01 mV/°C from -5 to 20°C and from 25 to 50°C
mV thermal drift:	-1999 ... +1999: ±0.05 mV/°C from -5 to 20°C and from 25 to 50°C
Noise 0 ÷ 10 Hz:	1 µV peak/peak
Simulation of compensation temperature:	-20 to 150°C (-4 to 302°F)
Output impedance:	100 KΩ 1%, 1 GΩ 5% (no leading load capacity)
Display:	LCD 2 lines, 3 ½ digits. Figure height approx. 12.5 mm.
Symbols:	pH, mV, °C, °F, HI imp., LO imp., 0.1 pH, 1 pH, 1 mV, 10 mV
Signals:	LOU, ER1, CAL
Working temperature:	-5 to 50°C (23 to 122°F)
Power supply:	9 Vdc alkaline battery. Low battery indication.
Consumption (instrument only):	5 mA lit, 20 µA off
Autonomy:	about 200 hours
Dimensions:	187 x 72 x 38 mm.
Weight:	300 gr

ORDER CODES

HD 9609: Kit composed of the instrument HD 9609, adapter cables CP 9509BNC, CP 9509 T, carrying case

CP 9509BNC: Adapter cable L = 1 mt, male BNC connector on both ends

CP 9509 T: Adapter cable L = 1 mt, BNC connector on only one end

CP9509S7: Adapter cable L = 1 mt, BNC wall connector one end, S7 male connector on the other end.

HD 9609 pH AND mV SIMULATOR

GENERAL CHARACTERISTICS

The simulator **HD 9609** is a portable instrument for checking and calibrating pH and mV measuring instruments. The characteristics of this instrument satisfy any checking and calibrating requirements for both portable and panel-mounted instruments; it may be used in laboratories, in industry or for checks in the field. Despite its many functions, the instrument is simple to use: a large display, with dual indication, and a series of symbols allow it to be used even by unskilled personnel.

The HD9609 sends to output in channel A the simulation of signals of an electrode for measuring pH, ORP, ISFET, in the range:

- 0 to 14 pH, with resolution 0.10 pH;
- ±1999 mV, with resolution 1 mV.

The user may choose between two output impedance values:

- 100 KΩ, low impedance;
- 1 GΩ, high impedance.

The simulation of the electrode compensation temperature is manually programmed in the range from -20°C to +150°C, while the temperature is measured in degrees Celsius or Fahrenheit.

The pH simulation values may be manually set as desired, in steps of 0.1 or 1 pH. The mV simulation values may be manually set as desired, in steps of 1 or 10 mV. The HD9609 is fed with an ordinary 9Vdc alkaline battery.

The electronics are housed in a sturdy ABS case with ergonomic lines.

In designing and making the instrument, each detail has been assessed and selected in order to provide an instrument with high performance and excellent long-term measurement stability.





DO 9403T-R1 pH/mV TRANSMITTER

The **DO 9403T-R1** pH transmitter converts the output of a pH electrode, with temperature compensation, into a signal at $4 \div 20$ mA. The pH or Redox electrode input circuit is galvanically insulated against the $4 \div 20$ mA output signal.

An LCD indicator allows viewing of the process signal value and of the various parameters. The accurate design and choice of components make the instrument precise and reliable for a long working life.

The instrument works with a pH or Redox electrode and a temperature probe (Pt100 sensor, 100Ω at 0°C).

Key functions

PRG Programming of the parameters is activated by pressing the PRG key. The Δ symbol lights up on the display and the message P1 appears, indicating that the parameter P1 is being programmed. When the PRG key is pressed continuously, the messages P2, P3, P4, P5, P6, P7, P8, P9, P10 and the corresponding parameters are displayed in sequence. After P10 the instrument returns to normal function.

After the parameter concerned has been displayed, it is possible to view its value by pressing the OK key. To change the parameter use the \blacktriangle and \blacktriangledown keys. Press the OK key again to confirm the value of the parameter.

SET Key for setting the relay intervention threshold. The Δ symbol and the REL symbol appear on the display, fixed or flashing, indicating the switching on or off threshold of relay A or of relay B.

$^\circ\text{C}/^\circ\text{F}$

- If this key is pressed it changes the temperature measuring unit to degrees Celsius or degrees Fahrenheit.
- When pressed together with the CAL key it activates the manual temperature setting function.
- If pressed during the pH calibration function it quits the calibration function without storing the calibration.

pH/mV

- If this key is pressed it changes the measuring unit to mV or pH.
- When pressed together with the CAL key it activates the pH calibration function.

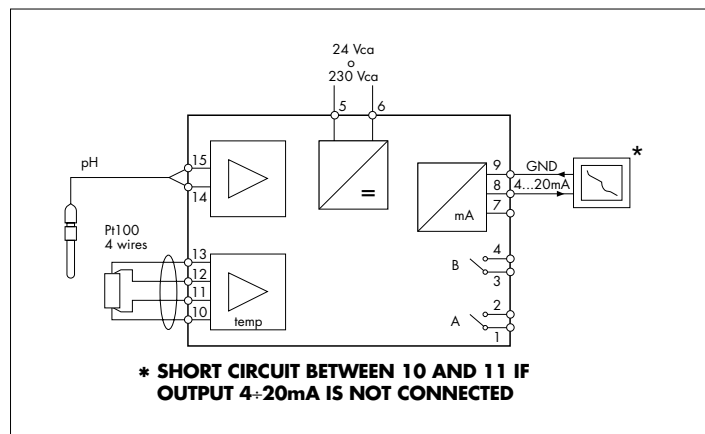


Fig.1 Active transmitter.

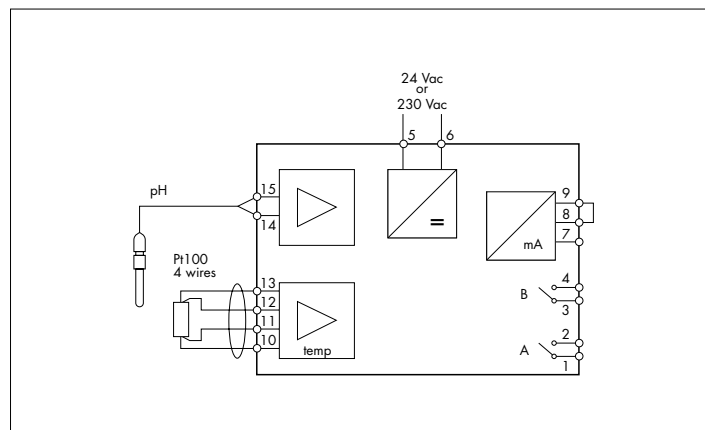


Fig.2 Active indicator.

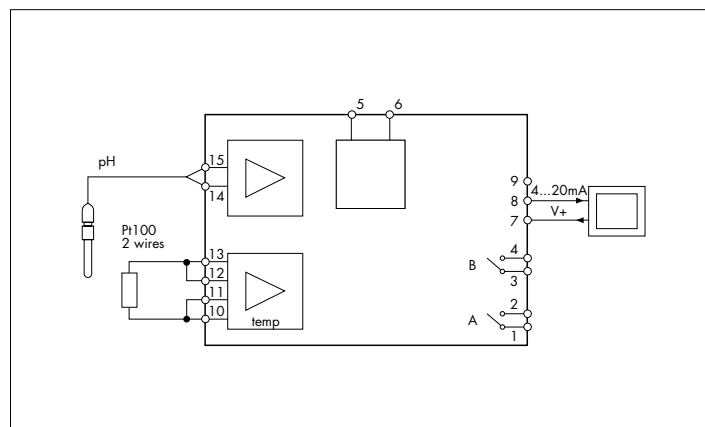


Fig.3 Passive transmitter.

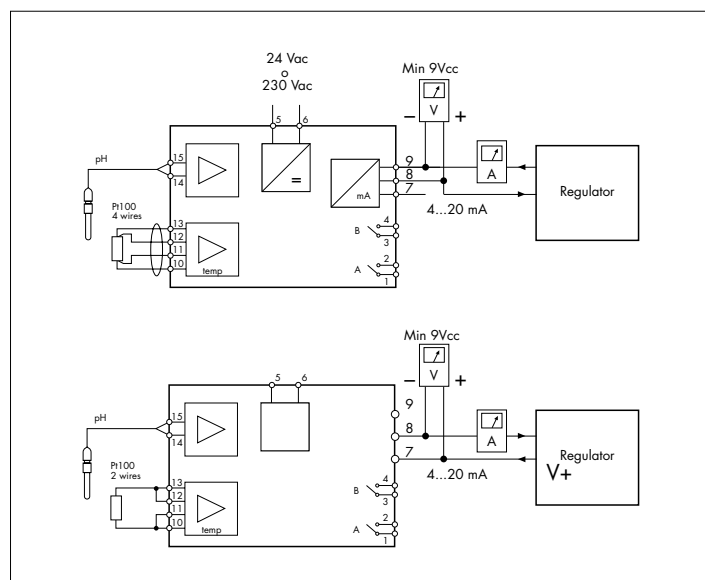


Fig.4

- OK** Confirms the programming parameters, or the relay SET values, and stores them.
- CAL**
- When pressed together with the °C/°F key it activates the manual temperature setting function.
 - When pressed together with the pH/mV key it activates the pH calibration function.
 - Key used to confirm pH calibration and manual temperature setting.
- ▲**
- Key for increasing the value displayed in the parameter programming phase.
 - During the relay SET point programming phase.
 - During the calibration phase.
- ▼**
- Key for decreasing the value displayed in the parameter programming phase.
 - During the relay SET point programming phase.
 - During the calibration phase.

Setting the relay SET point

- Press the SET button; the Δ symbol appears on the display.
- The REL symbol and the letter A also light up on the display to indicate that the value shown corresponds to the switching on threshold of relay A.
- To change this value press the ▲ and ▼ keys.
- Press SET; the REL symbol flashes and the letter A remains lit to indicate that the value shown corresponds to the switching off threshold of relay A.
- To change this value press the ▲ and ▼ keys.
- Press the SET button; the REL symbol and the letter B light up to indicate that the value shown corresponds to the switching off threshold of relay B.
- To change this value press the ▲ and ▼ keys.
- Press SET; the REL symbol flashes and the letter B remains lit to indicate that the value shown corresponds to the switching off threshold of relay B.
- To change this value press the ▲ and ▼ keys.
- Press SET, the instrument stores the set parameters and returns to normal function. The REL and Δ symbols disappear.

NOTE: During the SET point setting phase (REL symbol lit or flashing) the instrument returns to normal function if no key is pressed for 2 minutes.

Manual temperature setting

If the temperature probe is not connected or if the probe is broken the measuring unit °C or °F flashes. In this case it is possible to set the temperature compensation value manually.

- Press the CAL key and the °C/°F key together; the Δ symbol appears and the manual temperature is shown with the measuring unit flashing.
- Using the ▲ and ▼ keys, set the temperature value corresponding to the temperature of the liquid in which you wish to measure the pH.
- Press CAL to confirm this value. The Δ symbol switches off and the instrument returns to the previous display.


Calibration of the pH electrode

Calibration of the offset of the pH electrode:

- Immerse the electrode in the buffer solution used for calibrating the offset (6.86 pH).
- Press the CAL key and the pH/mV key together; the Δ symbol lights up on the display.
- Using the ▲ and ▼ keys, adjust the pH value measured as a function of the liquid temperature.
- Press CAL to confirm this value. The Δ symbol switches off.

Calibration of the slope of the pH electrode:

- Immerse the electrode in the buffer solution used for calibrating the slope (4.01 or 9.18 pH).
- Press the CAL key and the pH/mV key together; the Δ symbol lights up on the display.

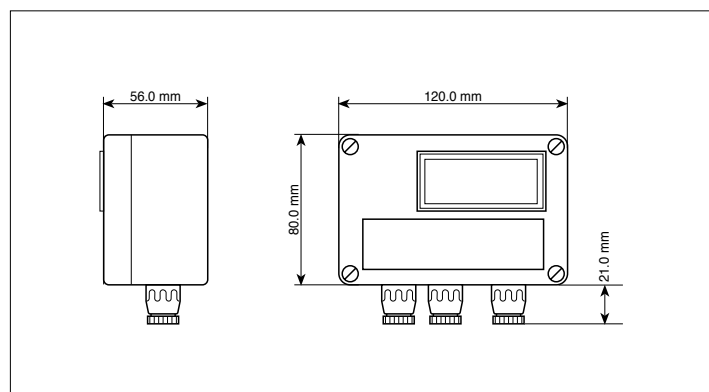

Dimensions

- Using the ▲ and ▼ keys, adjust the pH value measured as a function of the liquid temperature.
- Press CAL to confirm this value. The Δ symbol switches off.

NOTE: If you want to quit without storing the new calibration, press the °C/°F key. N.B.: The instrument can automatically recognize three standard calibration solutions: 4.01 pH, 6.86 pH and 9.18 pH.

Programming the parameters

- P1** Relay control unit and analog output, pH or mV.
- P2** pH/mV value corresponding to 4 mA at output. May be set between -1.00 pH and 15.00 pH or between -1999 mV and +1999 mV.
- P3** pH/mV value corresponding to 20 mA at output. May be set between -1.00 pH and 15.00 pH or between -1999 mV and +1999 mV.
- P4** Delay time in the intervention of relay A. May be set between 0 and 250 seconds.
- P5** Delay time in the intervention of relay B. May be set between 0 and 250 seconds.
- P6** Calibration of Pt100 probe.
- P7** 4 mA output current calibration.
- P8** 20 mA output current calibration.
- P9** Input voltage calibration.
- P10** Display of the offset voltage value and of the slope value of the electrode.

To change one of these parameters press key PRG until the message corresponding to the parameter to be changed appears on the screen.

Press OK to show the value of the parameter.

Using the ▲ and ▼ keys, bring the parameter displayed to the desired value.

Press OK again to confirm.

Parameter P10 cannot be altered, it can only be displayed.

NOTE **P6-P7-P8-P9: calibration procedure to be carried out at a laboratory by skilled workers.**

Pt100 probe calibration (100 Ω at 0°C)

- Connect the Pt100 probe to the instrument. Press the PRG key until the message P6 appears on the display.
- Press the OK key; the currently measured temperature appears on the display.
- Immerse the Pt100 probe and a precision thermometer for reference in the zero calibration bath. Wait long enough for the reading to become stable.

Combined electrode input	pH	-1.00 pH...15.00 pH (-500...+500 mV)
	ORP	-1999...+1999 mV
	Input impedance	>10 Tohm
	Cable length	<50 metres screened (about 5 nF)
	Accuracy	0.1% of reading ±1 digit ±0.01% of pH per °C of temperature drift
Temperature input	Pt100 2/4 wires	-50...199.9°C
	Transducer energizing	0.5 mA DC
	Cable length	<10 metres unscreened <20 metres screened (about 2 nF)
	Accuracy	0.2°C ±0.1% of reading ±2 digits ±0.01°C/°C
pH electrode temp. compensation	Automatic	According to Nerst
Current output	4.00...20.00 mA	Programmable and proportional to the pH or mV value
	Accuracy	0.5% of reading ±0.02 mA
	Insulation	2500 Vac 1 minute
Relay output	A and B	Bistable, contact 3 A/230 Vac free potential
Power supply	Active	24 or 230 Vac -15/+10% 1 VA, 48...62 Hz, see fig. 1
	Passive	4÷20 mA, 2 wire configuration, 10÷35 V, see fig. 2
Temp.	Operation	0...50°C
	Storage	-20...70°C, no condensation
Case	External dimensions	120x80x56 mm
	Protection class	IP64

- Using the ▲ and ▼ keys, adjust the value of the temperature measured by the Pt100 probe so that it corresponds with the value on the reference thermometer.
- Immerse the Pt100 probe and a precision thermometer in the full scale calibration bath. Wait long enough for the reading to become stable.
- Using the ▲ and ▼ keys, adjust the value of the temperature measured by the Pt100 probe so that it corresponds with the value on the reference thermometer.
- Press OK to confirm. To quit programming, press PRG repeatedly.

N.B.: If the temperature shown by the instrument is between $\pm 12^{\circ}\text{C}$, the instrument calibrates the probe offset, otherwise it calibrates the gain.

Calibrating the analog output

- Connect a precision milliammeter to the analog output.
- Press the PRG key until the message P7 appears on the display.
- Press OK; the message 4.0 appears on the display, indicating calibration at 4 mA.
- Using the ▲ and ▼ keys, adjust the value of the output current so as to have an indication of 4,00 mA on the precision milliammeter.
- Press the PRG key until the message P8 appears on the display.
- Press OK; the message 20.0 appears on the display, indicating calibration at 20 mA.
- Using the ▲ and ▼ keys, adjust the value of the output current so as to have an indication of 20,00 mA on the precision milliammeter.
- Press OK to confirm. To quit programming, press PRG repeatedly.

Calibrating the voltage input

- Press the PRG key until the message P9 appears on the display.
- Press OK; the mV value of the input appears on the display.
- Simulate a voltage of 0 mV at the input (if the value is between ± 25 mV the zero is calibrated, otherwise the full scale value is calibrated).
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Press the SET key, the REL symbol lights up on the display indicating that the instrument is measuring the voltage present at the input using the second measurement scale.
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Press the SET key, the REL symbol on the display switches off.
- Simulate a voltage of 450 mV at the input, corresponding to the full scale value of the first scale.
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Simulate a voltage of 1800 mV at the input, corresponding to the full scale value of the second scale.
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Press OK to confirm. To quit programming, press PRG repeatedly.

Display

Symbol	description
°C	indicates that the value shown is in °C.
°F	indicates that the value shown is in °F.
pH	indicates that the unit of the value shown is pH.
mV	Indicates that the unit of the value shown is milli Volts.
A	indicates that the relay A is in closed status.
B	indicates that the relay B is in closed status.
REL	<ul style="list-style-type: none"> - indicates that the value shown corresponds to the closing thresholds of the contacts of relay A or B; - indicates that the offset of the second voltage measurement scale is being calibrated.
REL flashing	indicates that the value shown corresponds to the opening thresholds of the contacts of relay A or B.
Δ	<ul style="list-style-type: none"> - indicates that the instrument is in the parameter setting phase; - indicates that the closing and opening thresholds of relays A and B are being changed; - indicates that the manual compensation temperature is being changed; - indicates that the pH electrode is being calibrated.

Error signals

- OFL** - Warning which appears during measurement when the value to be displayed is out of scale.
- E1** - Error warning which appears during pH calibration to indicate that the offset value of the electrode is too high in absolute value.
- E2** - Error warning which appears during pH calibration to indicate that the difference between the mV readings given by the two buffer solutions used for calibration is too great.
- E3** - Error warning which appears during pH calibration to indicate that the mV readings given by the two buffer solutions used for calibration are too close (about 50 mV at 25°C).
- E4** - Reading error on the EEPROM.
- E5** - Error warning indicating that the slope calculation gives a value 20% lower than the nominal value or gives a negative value.
- E6** - Error warning indicating that the slope calculation gives a value 150% lower than the nominal value.

Order code

- DO 9403T-R1:** pH transmitter 4÷20 mA passive or active, power supply 24 Vac, 120x80x56 mm for use in the field.
- HD 882 M100/300:** Temperature probe with Pt100 sensor, miniature head, shaft Ø 6x300 mm.
- HD 882 M100/600:** Temperature probe with Pt100 sensor, DIN B head, shaft Ø 6x600 mm.
- HD 8642:** Buffer solution 4.01 pH.
- HD 8672:** Buffer solution 6.86 pH.
- HD 8692:** Buffer solution 9.18 pH.
- HD 220:** Buffer solution redox 220 mV
- HD 468:** Buffer solution redox 468 mV
- HD62PT:** Diaphragm cleaning (tiourea in HCl) - 500ml.
- HD62PP:** Protein cleaning (pepsin in HCl) - 500ml.
- HD62RF:** Regeneration (fluorhydric acid) - 100ml.
- HD62SC:** Solution for electrode preservation - 200ml
- CP5:** Extension cable. Connector S/wire - TERMINAL BOARD.
- CP5/10:** Extension cable L=10m. Connector BNC/S7.
- CP5S:** Extension cable L=5m. Connector BNC/S7.
- CP5S/10:** Extension cable L=10m. Connector BNC/S7.
- KPI 10:** Combined industrial electrode, S7 brass 1" connector, glass body, Ag/AgCl sat KCl, Ø 12x120, temperature 0÷130°C, porous Teflon fitting.
- KPI 11:** Combined industrial electrode, S7 brass 1" connector, Rytron body, Ag/AgCl sat KCl, temperature 0÷100°C, porous Teflon fitting.
- KPI 12:** Platinum electrode for Redox measurement, S PG13,5 connector, pressure 6 bar.
- KPI 13:** Platinum electrode for Redox measurement, Rytron body, S PG13,5 connector, Ag/AgCl sat KCl.

Electrode dimensions at page 351



DO 9785T - DO 9765T pH TRANSMITTERS

DO 9785T/DO 9765T pH transmitters convert the output of a pH electrode, with temperature compensation, into a signal at 4÷20 mA. The pH electrode input circuit is galvanically insulated against the 4÷20 mA output signal.

An LCD indicator allows viewing of the process signal value and of the various parameters. The accurate design and choice of components make the instrument precise and reliable for a long working life.

The instrument works with a pH electrode or Redox and a temperature probe (Pt 100 sensor, 100 Ω at 0°C).

Technical characteristics

Combined electrode input	pH	-1,00 pH...15,00 pH (-500...+500 mV)
	ORP	-1999...+1999 mV
	Input impedance	>10 Tohm
	Cable length	<50 metres screened (about 5 nF)
	Accuracy	0.1% of reading ±1 digit ±0.01% pH per °C of drift in temperature
Temperature input	Pt100 2/4 wires	-50...199,9°C
	Transducer energizing	0,5 mA DC
	Cable length	<10 metres unscreened <50 metres screened (about 2 nF)
	Accuracy	0.2°C ±0.1% of reading ±2 digits ±0.01°C/°C
pH electrode compensation temperature	Automatic	According to Nernst
	Manual	-50÷200°C
Current output	4.00...20.00 mA	Programmable and proportional to the pH or mV value
	Accuracy	0.5% of reading ±0.02 mA
	Insulation	2500 Vac 1 minute
R Load	Load resistance	$R_{Lmax} = \frac{V_{dc}-10}{0,022}$ $R_{Lmax} = 636 \Omega @V_{dc} = 24 V_{dc}$
	Relay output	A and B Bistable, contact 3A/230 Vac free potential
Power supply	Passive	4÷20 mA, 2 wire configuration, 10÷35 V, see fig. 2
	Active	24 or 230 Vac - 15/+10% 1 VA, 48...62 Hz, see fig. 1
DO 9765T case	External dimensions	120x122x56 mm
	Protection class	IP64
DO 9785T case	External dimensions	96x96x126 mm
	Protection class	IP54

Key functions

PRG Programming of the parameters is activated by pressing the PRG key plus the ▲ and ▼ keys. The message P1 appears on the display, indicating that the parameter P1 is being programmed. When the PRG key is pressed continuously, the messages P2, P3, P4, P5, P6, P7 and the corresponding parameters are displayed in sequence. After P7 the instrument returns to normal function.

SET Key for setting the relay intervention threshold. The ON or OFF symbol appears on the display, indicating the switching on or off threshold of relay A or of relay B.

°C/°F

- If this key is pressed it changes the temperature measuring unit to degrees Celsius or degrees Fahrenheit.
- When pressed together with the CAL key it activates the manual temperature setting function.
- If pressed during the conductivity calibration function it quits the calibration function without storing the calibration.

pH/mV

- If this key is pressed it changes the measuring unit to mV or pH.
- When pressed together with the CAL key it activates the pH calibration function.

OK Confirms the programming parameters, or the relay SET values, and stores them.

CAL


- When pressed together with the °C/°F key it activates the manual temperature setting function.
- When pressed together with the pH/mV key it activates the pH calibration function.

▲

- Key used to confirm pH calibration and manual temperature calibration.
- Key for increasing the value displayed in the parameter programming phase.

▼

- During the relay SET point programming phase.
- During the calibration phase.
- Key for decreasing the value displayed in the parameter programming phase.
- During the relay SET point programming phase.
- During the calibration phase.

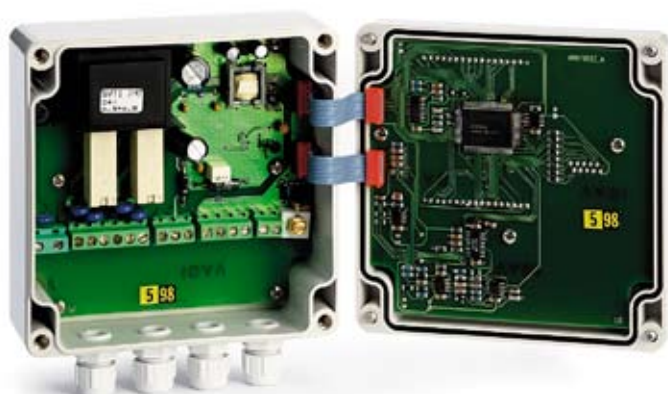

Setting the relay SET point

- Press the SET button; the ON symbol appears on the display with the letter A to indicate that the value shown corresponds to the switching on threshold of relay A.
- To change this value press the ▲ and ▼ keys.
- Press SET; the OFF symbol appears with the letter A to indicate that the switching off threshold of relay A is being displayed.
- To change this value press the ▲ and ▼ keys.
- Press the SET button; the ON symbol appears on the display with the letter B to indicate that the value shown corresponds to the switching on threshold of relay B.
- To change this value press the ▲ and ▼ keys.
- Press SET; the OFF symbol appears with the letter B to indicate that the switching off threshold of relay B is being displayed.
- To change this value press the ▲ and ▼ keys.
- Press SET, the instrument stores the values and returns to normal function.

NOTE: During the SET point setting phase (symbols ON or OFF lit) the instrument returns to normal function if no key is pressed for 2 minutes.

Temperature setting for manual compensation

If the temperature probe is not connected or if the probe is broken the measuring unit °C or °F flashes. In this case it is possible to set the temperature compensation value manually.

- Press the CAL key and the °C/°F key together; the message CAL appears at the bottom of the display.
- Using the ▲ and ▼ keys, set the temperature value corresponding to the temperature of the liquid in which you wish to measure the pH value.
- Press CAL to confirm this value. The message CAL disappears.

Calibration of the DO 9785T/DO 9765T with pH electrode

Calibration of the offset of the pH electrode:

- Immerse the electrode in the buffer solution used for calibrating the offset (6.86 pH).
- Press the CAL key and the pH/mV key together; the message CAL appears at the top of the display.
- Using the ▲ and ▼ keys, adjust the pH value measured as a function of the liquid temperature.
- Press CAL to confirm this value. The message CAL disappears.

Calibration of the slope of the pH electrode:

- Immerse the electrode in the buffer solution used for calibrating the slope (4.01 or 9.18 pH).
- Press the CAL key and the pH/mV key together; the message CAL appears at the top of the display.
- Using the ▲ and ▼ keys, adjust the pH value measured as a function of the liquid temperature.
- Press CAL to confirm this value. The message CAL disappears.

NOTE: If you want to quit without storing the new calibration, press the °C/°F key.

N.B.: The instrument can automatically recognize three standard calibration solutions: 4.01 pH, 6.86 pH and 9.18 pH.

Programming the parameters

- P1** Relay control unit and analog output, pH or mV.
- P2** pH/mV value corresponding to 4 mA at output. May be set between -1.00 pH and 15.00 pH or between -1999 mV and +1999 mV.
- P3** pH/mV value corresponding to 20 mA at output. May be set between -1.00 pH and 15.00 pH or between -1999 mV and +1999 mV.
- P4** Delay time in the intervention of relay A. May be set between 0 and 255 seconds.
- P5** Delay time in the intervention of relay B. May be set between 0 and 255 seconds.
- P6** Calibration of Pt100 probe, calibration of output in current, calibration of output in voltage. **(Calibration procedure to be carried out at a laboratory by skilled personnel).**
- P7** Display of the offset voltage value and of the slope value of the electrode.
- To change one of these parameters press key PRG until the message corresponding to the parameter to be changed appears on the screen. Using the ▼ and ▲ keys, bring the parameter displayed to the desired value. Press OK to confirm.
- Parameter P7 cannot be altered.**

Calibrating the voltage input (calibration procedure to be carried out at a laboratory by skilled workers)

- Press the PRG key until the message **P6** appears on the display.
- Press the **CAL key four times**; the message CAL appears at the top of the display and the mV value of the input at the bottom.
- Simulate a voltage of 0 mV at the input (if the value is between ±25 mV the zero is calibrated, otherwise the full scale value is calibrated).
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Press the **SET** button, the **ON** symbol appears on the display to indicate that the instrument is measuring the voltage of the input using the second scale of measurement.

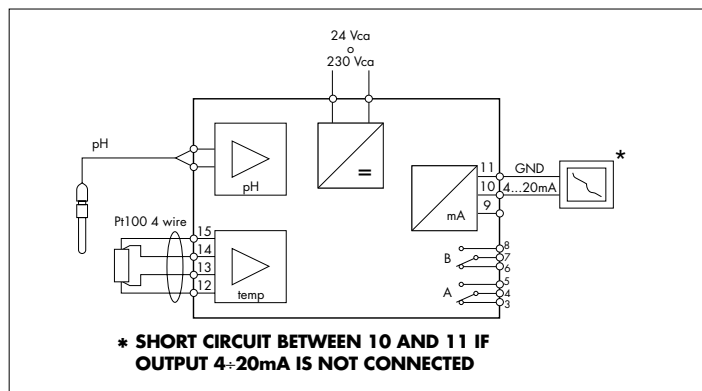


Fig.1 Active transmitter.

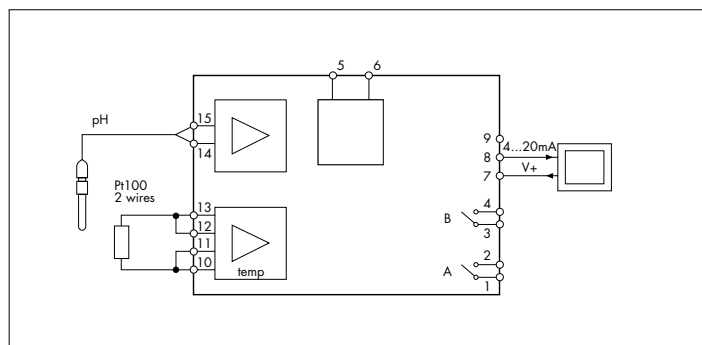


Fig.2 Passive transmitter.


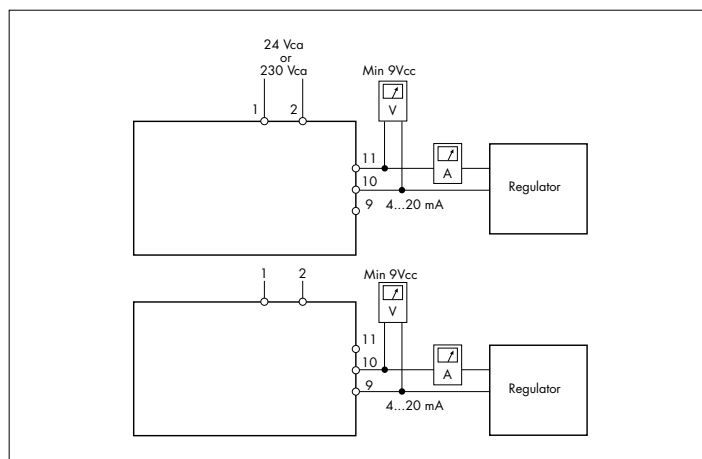


Fig.3

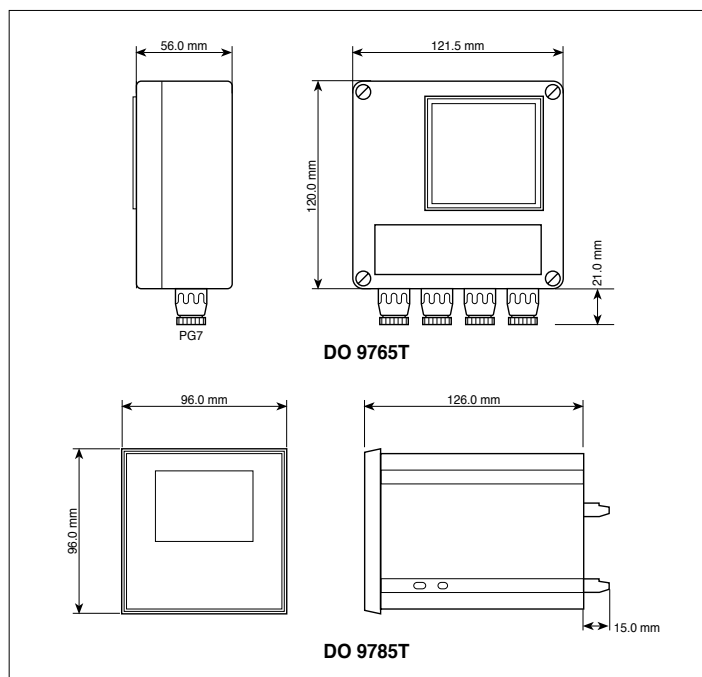

Dimensions

- Using the ▲ and ▼ keys adjust the voltage value so as to have the correct voltage value on the display.
- Press the set button, on the display the symbol **ON** disappears
- Simulate a voltage of 450 mV at the input, corresponding to the full value of the first scale.
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Simulate a voltage of 1800 mV at the input, corresponding to the full value of the second scale.
- Using the ▲ and ▼ keys, adjust the voltage value so as to have the correct voltage value on the display.
- Press OK to confirm.

Pt100 probe calibration (100 Ω at 0°C) (calibration procedure to be carried out at a laboratory by skilled workers)

- Connect the Pt100 probe to the instrument. Press the PRG key until the message **P6** appears on the display.
- Press the CAL key; the message CAL appears at the bottom of the display and the temperature is shown at the top.
- Immerse the Pt100 probe and a precision thermometer for reference in the zero calibration bath. Wait long enough for the reading to become stable.
- Using the ▲ and ▼ keys, adjust the value of the temperature measured by the Pt100 probe so that it corresponds with the value on the reference thermometer.
- Immerse the Pt100 probe and a precision thermometer in the full scale calibration bath. Wait long enough for the reading to become stable.
- Using the ▲ and ▼ keys, adjust the value of the temperature measured by the Pt100 probe so that it corresponds with the value on the reference thermometer.
- Press OK to confirm.

N.B.: If the temperature shown by the instrument is between $\pm 12^\circ\text{C}$, the instrument calibrates the probe offset, otherwise it calibrates the gain.

Calibrating the analog output (calibration procedure to be carried out at a laboratory by skilled workers)

- Press the PRG key until the message **P6** appears on the display.
- Connect a precision milliammeter to the analog output.
- Press the **CAL key twice**; the message CAL appears at the top of the display and the message 4.0 at the bottom, indicating calibration at 4 mA.
- Using the ▲ and ▼ keys, adjust the value of the output current so as to have an indication of 4.0 mA on the precision milliammeter.
- Press the CAL key; the message CAL appears at the top of the display and the message 20.0 at the bottom, indicating calibration at 20 mA.
- Using the ▲ and ▼ keys, adjust the value of the output current so as to have an indication of 20.0 mA on the precision milliammeter.
- Press OK to confirm.

Display

Symbol	description
°C	the value shown is in °C.
°F	the value shown is in °F.
pH	the unit of the value shown is pH.
mV	the unit of the value shown is milli Volts.
A	the relay A is in closed status.
B	the relay B is in closed status.
ON	the value shown corresponds to the closing thresholds of the contacts of relay A or B.
OFF	the value shown corresponds to the opening thresholds of the contacts of relay A or B.

Error signal

- OFL** - Warning which appears during measurement when the value to be displayed is out of scale.
- E1** - Error warning which appears during pH calibration to indicate that the offset value of the electrode is too high in absolute value.
- E2** - Error warning which appears during pH calibration to indicate that the difference between the mV readings given by the two buffer solutions used for calibration is too great.
- E3** - Error warning which appears during pH calibration to indicate that the mV readings given by the two buffer solutions used for calibration are too close (about 50 mV at 25°C).
- E4** - Reading error on the EEPROM.
- E5** - Error warning indicating that the slope calculation gives a value 20% lower than the nominal value or gives a negative value.
- E6** - Error warning indicating that the slope calculation gives a value 150% higher than the nominal value.

Order code

- DO 9785T**: pH transmitter 4÷20 mA passive or active, power supply 24 Vac with double display 96x96 mm, for panel mounting.
- DO 9765T**: pH transmitter 4÷20 mA passive or active, power supply 24 Vac with double display 122x120, for use on the field.
- HD 882 M100/300**: Temperature probe with Pt100 sensor, miniature head, shaft $\varnothing 6 \times 300$ mm.

HD 8642: Buffer solution 4.01 pH.

HD 8672: Buffer solution 6.86 pH.

HD 8692: Buffer solution 9.18 pH.

HDR 220: Buffer solution Redox 220 mV 0,5l.

HDR 468: Buffer solution Redox 468 mV 0,5l.

HD62PT: Diaphragm cleaning (tiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 200ml.

CP5/10: Extension cable for connecting the electrode to the DO9403T or to the DO9765T (S7-wire-TERMINAL BOARD) L=10m.

CP5: Extension for connecting the electrode to the DO 9403T-R1 or to the DO 9765T (S7-wire-TERMINAL BOARD) L=5m.

CP5S: Extension for connecting the electrode to the DO 9785T (BNC-S7) L=5m.


CP5S/10: Extension cable L=10m. Connector BNC/S7.

KPI 10: Combined industrial electrode, S7 PG13.5 connector, refillable, glass body, Ag/AgCl sat KCl $\varnothing 12 \times 120$ mm, temperature 0÷130°C, porous Teflon fitting.


KPI 11: Combined industrial electrode, S7 brass 1" connector, refillable, Rytron body, Ag/AgCl sat KCl, temperature 0÷100°C, porous Teflon fitting.

KPI 12: Platinum electrode for Redox measurement, S PG13,5 connector, pressure 6 bar.

KPI 13: Platinum electrode for Redox measurement, Rytron body, S PG13,5 connector, Ag/AgCl sat KCl.

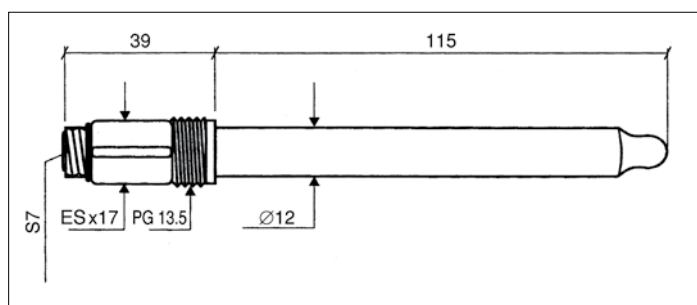

KPI 10 0...14 pH / KPI 12 Redox ± 1999 mV, 0...130°C

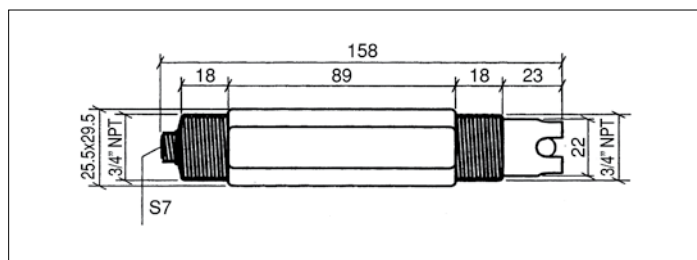

KPI 11 0...14 pH / KPI 13 Redox ± 1999 mV, 0...100°C





HD 2106.1, HD 2106.2 CONDUCTIVITY METERS - THERMOMETERS

The **HD2106.1** and **HD2106.2** are portable instruments with a large LCD display. They measure conductivity, liquid resistivity, total dissolved solids (TDS), and salinity using combined 4-ring and 2-ring conductivity/temperature probes. Temperature only is measured by Pt100 or Pt1000 immersion, penetration or contact probes.

The probe calibration can be performed automatically in one or more than one of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions.

The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside. The HD2106.2 is a **datalogger**. It memorizes up to 36,000 conductivity and temperature samples which can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing interval, printing, and baud rate can be configured using the menu. The HD2106.1 and HD2106.2 models are fitted with an RS232C serial port and can transfer to a PC the acquired measurements or to a portable printer in real time. The *Max*, *Min* and *Avg* function calculates the maximum, minimum or average values. Other functions include: the relative measurement REL, the Auto-HOLD function, and the automatic turning off which can also be excluded.

The instruments have IP67 protection degree.



HD40.1



SWD10

INSTRUMENT TECHNICAL CHARACTERISTICS

Measured quantities: χ , Ω , TDS, NaCl, °C, °F

Instrument

Dimensions (Length x Width x Height)	185x90x40mm
Weight	470g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ digits plus symbols
Visible area:	52x42mm

Operating conditions

Working temperature	-5...50°C
Storage temperature	-25...65°C
Working relative humidity	0...90%RH without condensation
Protection degree	IP67

Power

Batteries	4 1.5V type AA batteries
Autonomy	200 hours with 1800mAh alkaline batteries
Power absorbed with instrument off	20µA
Mains	Output mains adapter 12Vdc / 1A

Security of memorized data

Unlimited, independent of battery charge conditions

Time

Date and time	Schedule in real time
Accuracy	1min/month max error

Measured values storage - model **HD2106.2**

Type	2000 pages containing 18 samples each
Quantity	36000 pairs of measurements [χ -°C], [Ω -°C], [TDS-°C] or [Sal-°C]
Selectable storage interval	1s, 5s, 10s, 15s, 30s, 60s (1min), 120s (2min), 300s (5min), 600s (10min), 900s (15min), 1200s (20min), 1800s (30min) and 3600s (1hour)

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Selectable print interval	1s, 5s, 10s, 15s, 30s, 60s (1min), 120s (2min), 300s (5min), 600s (10min), 900s (15min), 1200s (20min), 1800s (30min) and 3600s (1hour)

USB interface - model **HD2106.2**

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Connections

Conductivity input	8-pole male DIN45326 connector
Input module for the temperature probes	8-pole male DIN45326 connector
Serial interface and USB	8-pole MiniDin connector
Mains adapter	2-pole connector (positive at centre)

Measurement of conductivity

Measuring range		Resolution
Kcell=0.1	0.00...19.99µS/cm	0.01µS/cm
Kcell=1	0.0...199.9µS/cm	0.1µS/cm
	200...1999µS/cm	1µS/cm
	2.00...19.99mS/cm	0.01mS/cm
	20.0...199.9mS/cm	0.1mS/cm
	200...1999mS/cm	1mS/cm
Measuring range		
Kcell=10		
Accuracy (conductivity)	±0.5%1 digit	

Measurement of resistivity

Measuring range Kcell=0.1	till 100MΩ·cm/(*)
Measuring range Kcell=1	5.0...199.9Ω·cm 200...999Ω·cm 1.00k...19.99kΩ·cm 20.0k...99.9kΩ·cm 100k...999kΩ·cm 1...10MΩ·cm
Measuring range Kcell=10	0.5...5.0Ω·cm
Accuracy (resistivity)	±0.5%±1 digit

Resolution

0.1Ω·cm
1Ω·cm
0.01kΩ·cm
0.1kΩ·cm
1kΩ·cm
1MΩ·cm
0.1Ω·cm

Temperature compensation

automatic/manual

Reference temperature
X / TDS Conversion factor
Cell constant K (cm⁻¹)

0...100°C with α_T selectable from 0.00 to 4.00%/°C
20°C or 25°C
0.4...0.8
0.1, 0.7, 1.0 and 10.0

Standard solutions automatically detected @25°C

147μS/cm
1413μS/cm
12880μS/cm
111800μS/cm

Measurement of total dissolved solids (with coefficient X/TDS=0.5)

Measuring range Kcell=0.1	0.00...19.99mg/l	0.05mg/l
Measuring range Kcell=1	0.0...199.9mg/l 200...1999mg/l 2.00...19.99g/l 20.0...99.9g/l	0.5mg/l 1mg/l 0.01g/l 0.1g/l
Measuring range Kcell=10	100...999g/l	1g/l
Accuracy (conductivity)	±0.5%1 digit	

Preset cell constant values:

K=0,01 - K=0,1 - K=1, K=10

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity (μS/cm)	Resistivity (MΩ·cm)	Conductivity (μS/cm)	Resistivity (MΩ·cm)
0.001 μS/cm	1000 MΩ·cm	0.01 μS/cm	100 MΩ·cm
0.002 μS/cm	500 MΩ·cm	0.02 μS/cm	50 MΩ·cm
0.003 μS/cm	333 MΩ·cm	0.03 μS/cm	33 MΩ·cm
0.004 μS/cm	250 MΩ·cm	0.04 μS/cm	25 MΩ·cm
...

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

Measurement of salinity

Measurement range	0.000...1.999g/l 2.00...19.99g/l 20.0...199.9g/l	Resolution 1 mg/l 10mg/l 0.1g/l
Accuracy (salinity)	±0.5%1 digit	

Measurement of temperature

Pt100 measuring range	-50...+200°C
Pt1000 measuring range	-50...+200°C
Resolution	0.1°C
Accuracy	±0.25°C
Drift after 1 year	0.1°C/year

4 wire Pt100 and 2 wire Pt1000 Temperature probes

Model	Type	Working range	Accuracy
TP47.100	Pt100 4 wires	-50...+200°C	Class A
TP47.1000	Pt1000 2 wires	-50...+200°C	Class A
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @20°C

0.005%/°C



ORDER CODES

HD2106.1: The kit is composed of: instrument HD2106.1, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software.

HD2106.2: The kit is composed of: instrument HD2106.2 **datalogger**, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software.

Conductivity probes, temperature probes, standard calibration solutions, cables for data transfer to PC or printer have to be ordered separately.

HD2110CSNM: 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

C.206: Serial connection cable with USB connector for PC and 8-pole MiniDin male connector for the instrument

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole MiniDin (not suitable for HD2106.1K).

DeltaLog9: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply 100-240 Vac/12Vdc-1A mains voltage

HD40.1: 24-column portable thermal printer, serial interface, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm in diameter.

BAT-40: Spare battery pack for HD40.1 printer with built-in temperature sensor.

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by bench-top meters of the series HD22...with cable HD22.2.1 (optional) or power supplier SWD10 (optional).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147 μ S/cm @25°C, 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413 μ S/cm @25°C, 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880 μ S/cm @25°C, 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800 μ S/cm @25°C, 200cc.

Temperature probes complete with SICRAM module

TP87: Pt100 sensor immersion probe. Stem \varnothing 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem \varnothing 3 mm, length 230 mm. Cable length 2 m.

TP473P0: Pt100 sensor penetration probe. Stem \varnothing 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem \varnothing 4mm, length 230mm, contact surface \varnothing 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem \varnothing 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem \varnothing 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem \varnothing 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP87.100: Pt100 sensor immersion probe. Probe's stem \varnothing 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem \varnothing 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.






TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes

Conductivity probes

Please see the order codes reported in the probes' technical specifications.

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT

2 and 4 electrode conductivity probes

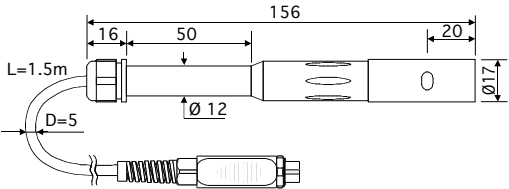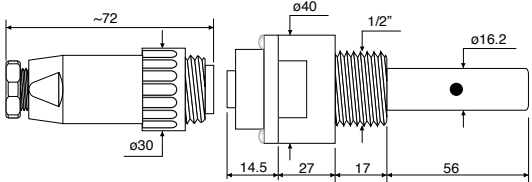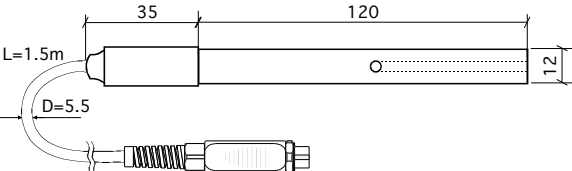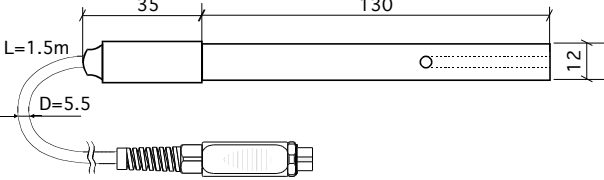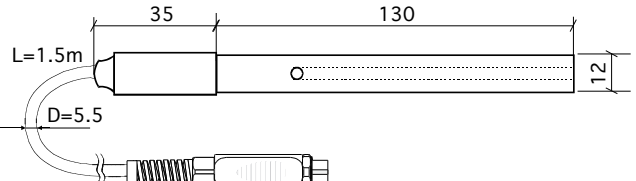ORDER CODE	MEASUREMENT RANGE	DIMENSIONS
SP06T	K=0.7 5 μ S...200mS/cm 0...90°C 4-electrode cell in Pocan/Platinum	
SPT 400.001 not suitable for HD 2306.0	K=0.01 0,05...19,9 μ S/cm 2-electrode cell AISI 316 - Teflon	
SPT01G	K=0.1 0.1 μ S...500 μ S/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT1G	K=1 10 μ S...10mS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT10G	K=10 500 μ S...200mS/cm 0...80°C 2-electrode cell in Glass/Platinum	



HD 2306.0 CONDUCTIVITY METER - THERMOMETER

The **HD2306.0** is a portable instrument with a large LCD display. It measures conductivity, liquid resistivity, total dissolved solids (TDS), and salinity using combined 4-ring and 2-ring conductivity/temperature probes. Temperature only is measured by Pt100 or Pt1000 immersion, penetration or contact probes. The probe calibration can be performed automatically in one or more than one of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

The *Max*, *Min* and *Avg* function calculates the maximum, minimum or average values. Other functions include: the relative measurement REL, the Auto-HOLD function, and the automatic turning off which can also be disabled.

The instrument has IP67 protection degree.

INSTRUMENT TECHNICAL CHARACTERISTICS

Measured quantities: χ , Ω , TDS, °C, °F

Instrument

Dimensions

(Length x Width x Height)

Weight

Materials

Display

140x88x38mm

160g (complete with batteries)

ABS

2x4½ digits plus symbols

Visible area: 52x42mm

Operating conditions

Working temperature

Storage temperature

Working relative humidity

Protection degree

-5...50°C

-25...65°C

0...90%RH without condensation

IP67

Power

Batteries

Autonomy

Power absorbed with instrument off

3 1.5V type AA batteries

200 hours with 1800mAh alkaline batteries

< 20µA

Connections

Conductivity input/temperature probes 8-pole male DIN45326 connector

Measurement of conductivity

Measuring range	0.00...19.99µS/cm	Resolution	0.01µS/cm
Kcell=0.1			
Measuring range	0.0...199.9µS/cm		0.1µS/cm
Kcell=1	200...1999µS/cm		1µS/cm
	2.00...19.99mS/cm		0.01mS/cm
	20.0...199.9mS/cm		0.1mS/cm
Measuring range	200...1999mS/cm		1mS/cm
Kcell=10			
Accuracy (conductivity)	±0.5%1digit		

Measurement of resistivity

Measuring range	till 100MΩ·cm/(*)		
Kcell=0.1			
Measuring range	5.0...199.9Ω·cm		0.1Ω·cm
Kcell=1	200...999Ω·cm		1Ω·cm
	1.00k...19.99kΩ·cm		0.01kΩ·cm
	20.0k...99.9kΩ·cm		0.1kΩ·cm
	100k...999kΩ·cm		1kΩ·cm
	1...10MΩ·cm		1MΩ·cm
Measuring range	0.5...5.0Ω·cm		0.1Ω·cm
Kcell=10			
Accuracy (resistivity)	±0.5%±1digit		

Measurement of salinity

Measurement range	0.000...1.999g/l	Resolution	1mg/l
	2.00...19.99g/l		10mg/l
	20.0...199.9g/l		0.1g/l
Accuracy (salinity)	±0.5%1digit		

Measurement of total dissolved solids (with coefficient χ /TDS=0.5)

Measuring range	0.00...19.99mg/l		0.05mg/l
Kcell=0.1			
Measuring range	0.0...199.9mg/l		0.5mg/l
Kcell=1	200...1999mg/l		1mg/l
	2.00...19.99g/l		0.01g/l
	20.0...99.9g/l		0.1g/l
Measuring range	100...999g/l		1g/l
Kcell=10			
Accuracy (conductivity)	±0.5%±1digit		

Measurement of temperature

Pt100 measuring range	-50...+200°C
Pt1000 measuring range	-50...+200°C
Resolution	0.1°C
Accuracy	±0.25°C
Drift after 1 year	0.1°C/year

Temperature compensation automatic/manual

0...100°C with α_t selectable from 0.00 to 4.00%/°C

Reference temperature 20°C or 25°C

χ / TDS Conversion factor 0.4...0.8

Cell constant K (cm⁻¹) 0.1, 0.7, 1.0 and 10.0

Standard solutions automatically detected @25°C

147µS/cm

1413µS/cm

12880µS/cm

111800µS/cm

Preset cell constant values:

K=0,01 - K=0,1 - K=1, K=10



(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.1 cm ⁻¹	
Conductivity (µS/cm)	Resistivity (MΩ·cm)
0.01 µS/cm	100 MΩ·cm
0.02 µS/cm	50 MΩ·cm
0.03 µS/cm	33 MΩ·cm
0.04 µS/cm	25 MΩ·cm

4 wire Pt100 and 2 wire Pt1000 Temperature probes

Model	Type	Working range	Accuracy
TP47.100	Pt100 4 wires	-50...+200°C	Class A
TP47.1000	Pt1000 2 wires	-50...+200°C	Class A
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @20°C 0.005%/°C

ORDER CODES

HD2306.0K: The kit is composed of: instrument HD2306.0, 3 1.5V alkaline batteries, operating manual, case. **Other conductivity probes, temperature probes, calibration solutions must be ordered separately.**

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by bench-top meters of the series HD22...with cable HD22.2.1 (optional) or power supplier SWD10 (optional).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

Conductivity probes

Please see the order codes reported in the probes' technical specifications.

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147µS/cm @25°C, 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413µS/cm @25°C, 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880µS/cm @25°C, 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800µS/cm @25°C, 200cc.

Temperature probes complete with SICRAM module

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD8747

HD8714

HD8712

HD8711

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT

2 and 4 electrode conductivity probes

ORDER CODE	MEASUREMENT RANGE	DIMENSIONS
SP06T	K=0.7 5µS...200mS/cm 0...90°C 4-electrode cell in Poca/Platinum	
SPT01G	K=0.1 0.1µS...500µS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT1G	K=1 10µS...10mS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT10G	K=10 500µS...200mS/cm 0...80°C 2-electrode cell in Glass/Platinum	



HD 2156.1 E HD 2156.2 pH METER - CONDUCTIVITY METER - THERMOMETER

The **HD2156.1** and **HD2156.2** are portable instruments with a large LCD display. They measure pH, mV, redox potential (ORP), conductivity, liquid resistivity, total dissolved solids (TDS) and salinity using combined 4-ring and 2-ring conductivity/temperature probes. Temperature only is measured by Pt100 or Pt1000 immersion, penetration or contact probes.

The pH electrode calibration, as well as manual, can be carried out on one, two or three points and the calibration sequence can be chosen from a list of 13 buffers. The probe calibration can be performed automatically in one or more of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions.

The HD2156.2 instrument is a **datalogger**. It stores up to 20,000 sets of three measurements composed of pH or mV, conductivity or resistivity or TDS or salinity and temperature: these data can be transferred to a PC from the instrument connected via the multi-standard RS232C serial port and USB 2.0. The storing interval, printing, and baud rate can be configured using the menu.

The HD2156.1 and HD2156.2 models are fitted with an RS232C serial port and can transfer the acquired measurements to a PC or to a portable printer in real time.

The *Max*, *Min* and *Avg* function calculates the maximum, minimum or average values.

Other functions include: the Auto-HOLD function and the automatic turning off which can also be excluded.

The instruments have IP67 protection degree.

INSTRUMENT TECHNICAL CHARACTERISTICS

Measured quantities: pH, mV, χ , Ω , TDS, NaCl, °C, °F

Instrument

Dimensions (Length x Width x Height)	185x90x40mm
Weight	470g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ digits plus symbols Visible area: 52x42mm

Operating conditions

Working temperature	-5...50°C
Storage temperature	-25...65°C
Working relative humidity	0...90%RH without condensation
Protection degree	IP67

Power

Batteries	4 1.5V type AA batteries
Autonomy	200 hours with 1800mAh alkaline batteries
Power absorbed with instrument off	20µA
Mains (SWD10)	Output mains adapter 12Vdc / 1A
Security of memorized data	Unlimited, independent of battery charge conditions

Time

Date and time	Schedule in real time
Accuracy	1min/month max error

Measured values storage - model **HD2156.2**

Type	2000 pages containing 10 samples each
Quantity	20,000 sets of three measurements composed of pH or mV, χ or Ω or TDS or salinity and temperature.
Selectable storage interval	1s, 5s, 10s, 15s, 30s, 60s (1min), 120s (2min), 300s (5min), 600s (10min), 900s (15min), 1200s (20min), 1800s (30min) and 3600s (1hour)

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Selectable print interval	1s, 5s, 10s, 15s, 30s, 60s (1min), 120s (2min), 300s (5min), 600s (10min), 900s (15min), 1200s (20min), 1800s (30min) and 3600s (1hour)

USB interface - model **HD2156.2**

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Connections

pH/mV input	Female BNC connector
Conductivity input	8-pole male DIN45326 connector
Serial interface and USB	8-pole MiniDin connector
Mains adapter	2-pole connector (positive at centre)

Measurement of pH by Instrument

Measurement range	-2.000...+19.999pH
Resolution	0.01 or 0.001pH selectable from menu
Accuracy	±0.001pH ±1digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	Offset! > 20mV Slope > 63mV/pH or Slope < 50mV/pH Sensitivity > 106.5% or Sensitivity < 85%

Measurement of mV by Instrument

Measurement range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	±0.1mV ±1digit
Drift after 1 year	0.5mV/year

Measurement of conductivity			Measurement of salinity		
Measuring range	0.00...19.99µS/cm	Resolution 0.01µS/cm	Measurement range	0.000...1.999g/l	Resolution 1mg/l
Kcell=0.1				2.00...19.99g/l	10mg/l
Measuring range	0.0...199.9µS/cm	0.1µS/cm	Accuracy (salinity)	20.0...199.9g/l	0.1g/l
Kcell=1	200...1999µS/cm	1µS/cm		±0.5%1digit	
	2.00...19.99mS/cm	0.01mS/cm			
	20.0...199.9mS/cm	0.1mS/cm	Temperature compensation		
Measuring range	200...1999mS/cm	1mS/cm	automatic/manual		
Kcell=10			0...100°C with αT selectable from 0.00 to 4.00%/°C		
Accuracy (conductivity)	±0.5%1digit		Reference temperature		
			20°C or 25°C		
Measurement of resistivity			χ / TDS Conversion factor		
Measuring range	till 100MΩ·cm/(*)	Resolution	0.4...0.8		
Kcell=0.1			Cell constant K (cm⁻¹)		
Measuring range	5.0...199.9Ω·cm	0.1Ω·cm	0.1, 0.7, 1.0 and 10.0		
Kcell=1	200...999Ω·cm	1Ω·cm	Standard solutions automatically detected @25°C		
	1.00k...19.99kΩ·cm	0.01kΩ·cm	147µS/cm		
	20.0k...99.9kΩ·cm	0.1kΩ·cm	1413µS/cm		
	100k...999kΩ·cm	1kΩ·cm	12880µS/cm		
	1...10MΩ·cm	1MΩ·cm	111800µS/cm		
Measuring range	0.5...5.0Ω·cm	0.1Ω·cm	Measurement of temperature		
Kcell=10			Pt100 measuring range		
Accuracy (resistivity)	±0.5%±1digit		-50...+200°C		
			Pt1000 measuring range		
Measurement of total dissolved solids (with coefficient χ/TDS=0.5)			-50...+200°C		
Measuring range	0.00...19.99mg/l	0.05mg/l	Resolution		
Kcell=0.1			0.1°C		
Measuring range	0.0...199.9mg/l	0.5mg/l	Accuracy		
Kcell=1	200...1999mg/l	1mg/l	±0.25°C		
	2.00...19.99g/l	0.01g/l	Drift after 1 year		
	20.0...99.9g/l	0.1g/l	0.1°C/anno		
Measuring range	100...999g/l	1g/l	Preset cell constant values:		
Kcell=10			K=0,01 - K=0,1 - K=1, K=10		
Accuracy (conductivity)	±0.5%1digit				

The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity (µS/cm)	Resistivity (MΩ·cm)	Conductivity (µS/cm)	Resistivity (MΩ·cm)
0.001 µS/cm	1000 MΩ·cm	0.01 µS/cm	100 MΩ·cm
0.002 µS/cm	500 MΩ·cm	0.02 µS/cm	50 MΩ·cm
0.003 µS/cm	333 MΩ·cm	0.03 µS/cm	33 MΩ·cm
0.004 µS/cm	250 MΩ·cm	0.04 µS/cm	25 MΩ·cm

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT

2 and 4 electrode conductivity probes

ORDER CODE	MEASUREMENT RANGE	DIMENSIONS
SP06T	K=0.7 5µS...200mS/cm 0...90°C 4-electrode cell in POCAN/Platinum	
SPT 400.001 not suitable for HD 2306.0	K=0.01 0,05...19,9µS/cm 2-electrode cell AlSi 316 - Teflon	
SPT01G	K=0.1 0.1µS...500µS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT1G	K=1 10µS...10mS/cm 0...80°C 2-electrode cell in Glass/Platinum	
SPT10G	K=10 500µS...200mS/cm 0...80°C 2-electrode cell in Glass/Platinum	

Temperature probes with 4 wire Pt100 and 2 wire Pt1000 connector sensor

Model	Type	Working range	Accuracy
TP47.100	Pt100 4 wires	-50...+200°C	Class A
TP47.1000	Pt1000 2 wires	-50...+200°C	Class A
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @20°C 0.005%/°C

ORDER CODES

HD2156.1: The kit is composed of: instrument HD2156.1, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software.

HD2156.2: The kit is composed of: instrument HD2156.2 **datalogger**, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software.

pH/mV probes, conductivity probes, temperature probes, standard calibration solutions for various types of measurements, connection cables for pH electrodes with S7 connector, cables for data transfer to PC or printer have to be ordered separately.

HD2110CSNM: 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

C.206: Serial connection cable with USB connector for PC and 8-pole MiniDin male connector for the instrument

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole MiniDin (not suitable for HD2156.1K).

DeltaLog9: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply 100-240 Vac/12Vdc-1A mains voltage

HD40.1: 24-column portable thermal printer, serial interface, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm in diameter.

BAT-40: Spare battery pack for HD40.1 printer with built-in temperature sensor.

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by bench-top meters of the series HD22...with cable HD22.2.1 (optional) or power supplier SWD10 (optional).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

pH Electrodes

KP 20: Gel pH filled combined electrode for general use, with S7 screw connector, EPOXY body.

KP 30: Gel pH combined electrode for general use, 1m cable with BNC, EPOXY body.

KP 50: Gel pH combined electrode, porous Teflon ring junction, suitable for emulsions, demineralised water, with S7 screw connector, glass body.

KP 61: 3 diaphragm liquid filled pH combined electrode for wine, milk, cream, etc., S7 screw connector, liquid reference filling, glass body.

KP 62: 1 diaphragm gel pH combined electrode for pure water, varnishes, gel filled, S7 screw connector, glass body.

KP 63: 1 liquid filled pH combined electrode for general use, varnishes, 1m cable with BNC, glass body.

KP 64: Liquid filled pH combined electrode, Teflon ring diaphragm, for wine, varnishes, emulsions, S7 screw connector, glass body.

KP 70: Pointed gel combined pH microelectrode diam. 6 x L=70 mm., with S7 screw connector, EPOXY body, glass tip, open junction.

KP 80: Pointed gel pH combined electrode, with S7 screw connector, glass body, for cream, milk, viscous material, open junction.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

Characteristics and dimensions of the probes at page 401

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP: 1.5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 5: 5m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 10: 10m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CP 15: 15m extension cable with BNC/S7 connector for electrode without cable, thread S7.

CE: S7 screw connector for pH electrode.

BNC: female BNC for extension cable

ORP Electrodes

KP 90: REDOX PLATINUM liquid filled electrode with S7 screw connector, glass body.

KP 91: Gel REDOX PLATINUM electrode, 1m cable with BNC, EPOXY body

Characteristics and dimensions of the probes at page 402

pH Buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox Buffer solutions

HDR220: Redox buffer solution 220mV 0.5 l.

HDR468: Redox buffer solution 468mV 0.5 l.

Electrolyte solutions

KCL3M Ready to use solution for electrode refilling - 100 cc

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fl uorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 200ml.

Conductivity probes

See order codes reported in the table at page 358.

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001 mol/l equal to 147µS/cm @25°C, 200cc.

HD8714: Standard calibration solution 0.01 mol/l equal to 1413µS/cm @25°C, 200cc.

HD8712: Standard calibration solution 0.1 mol/l equal to 12880µS/cm @25°C, 200cc.

HD87111: Standard calibration solution 1 mol/l equal to 111800µS/cm @25°C, 200cc.

Temperature probes complete with SICRAM module

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP472I.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP472I.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP472I.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.





DO 9786T - R1 • DO 9766T - R1

CONDUCTIVITY TRANSMITTERS

DO 9786T/DO 9766T transmitters convert the output of a conductivity electrode with temperature compensation into a 4÷20 mA signal.

The electrode input circuit is galvanically insulated against the 4÷20 mA output signal. An LCD indicator allows viewing of the process signal value and of the various parameters. The accurate design and choice of components make the instrument precise and reliable for a long working life.

The instrument works in conjunction with a conductivity electrode and a temperature probe (Pt100 sensor, 100 Ω at 0°C).

Technical characteristics

Input conductivity	Measuring range	0.0...199.9 mS
	2/4 electrodes	Configurable cell constant 0.01...199.9 cm-1
	Transducer energizing	Square wave 10...1000 mV, depending on conductivity, 200...1600 Hz, depending on conductivity
	Input impedance	>100 Mohm
	Cable length	<10 metres unscreened <50 metres screened (about 2 nF)
	Accuracy	0.5% of reading ±2 digits ±0.01% per °C of drift in temperature
Input temperature	Pt100 2/4 wires	-50...199.9°C
	Transducer energizing	0.5 mA dc
	Cable length	<10 metres unscreened <50 metres screened (about 5 nF)
	Accuracy	0.2°C ±0.1% of reading ±0.01°C/°C of drift in temperature
	Reference temperature	20 or 25°C Configurable
Compensation temperature	None	
	manual	Linear 0.00...4.00%/°C -50...+200C
	automatic	Linear 0.00...4.00%/°C -50...+200C
	Reference temperature	20 or 25°C Configurable
Current output	4.00...20.00 mA	Programmable and proportional to conductivity
	Accuracy	0.5% of reading ±0.02 mA
	Insulation	2500 Vac 1 minute
Relay output	A and B	Bistable, contact 3A/230 Vac free potential
Power supply	Passive	4÷20 mA, 2 wire configuration, 10÷35 V, see fig. 2
	Active	24/230 Vac - 15/+10% 1 VA, 48...62 Hz, see fig. 1
Case DO 9766T	External dimensions	120x122x56 mm
	Protection class	IP64
Case DO 9786T	External dimensions	96x96x126 mm
	Protection class	IP44


Key functions

- PRG** Programming of the parameters is activated by pressing the PRG key plus the ▲ and ▼ keys. The message P1 appears on the display, indicating that the parameter P1 is being programmed. When the PRG key is pressed continuously, the messages P2, P3, P4, P5, P6, P7, P8 and the corresponding parameters are displayed in sequence. After P8 the instrument returns to normal function.
- SET** Key for setting the relay intervention threshold. The ON or OFF symbol appears on the display, indicating the switching on or off threshold of relay A or of relay B.
- °C/°F** - If this key is pressed it changes the temperature measuring unit to degrees Celsius or degrees Fahrenheit.
- When pressed together with the CAL key it activates the manual temperature setting function.
- If pressed during the conductivity calibration function it quits the calibration function without storing the calibration.
- X** When pressed together with the CAL key it activates the conductivity calibration function.
- OK** Confirms the programming parameters, or the relay SET values, and stores them.
- CAL** - When pressed together with the °C/°F key it activates the manual temperature setting function.
- When pressed together with the X key it activates the conductivity calibration function.
- Key used to confirm conductivity calibration and manual temperature calibration.
- ▲ - Key for increasing the value displayed in the parameter programming phase.
- During the relay SET point programming phase.
- During the calibration phase.
- ▼ - Key for decreasing the value displayed in the parameter programming phase.
- During the relay SET point programming phase.
- During the calibration phase.

Setting the relay SET point

- Press the SET button; the ON symbol appears on the display with the letter A to indicate that the value shown corresponds to the switching on threshold of relay A.
- To change this value press the ▲ and ▼ keys.
- Press SET; the OFF symbol appears with the letter A to indicate that the switching off threshold of relay A is being displayed.
- To change this value press the ▲ and ▼ keys.
- Press the SET button; the ON symbol appears on the display with the letter B to indicate that the value shown corresponds to the switching on threshold of relay B.
- To change this value press the ▲ and ▼ keys.
- Press SET; the OFF symbol appears with the letter B to indicate that the switching off threshold of relay B is being displayed.
- To change this value press the ▲ and ▼ keys.
- Press SET, the instrument stores the values and returns to normal function.

NOTE: During the SET point setting phase (symbols ON or OFF lit) the instrument returns to normal function if no key is pressed for 2 minutes.

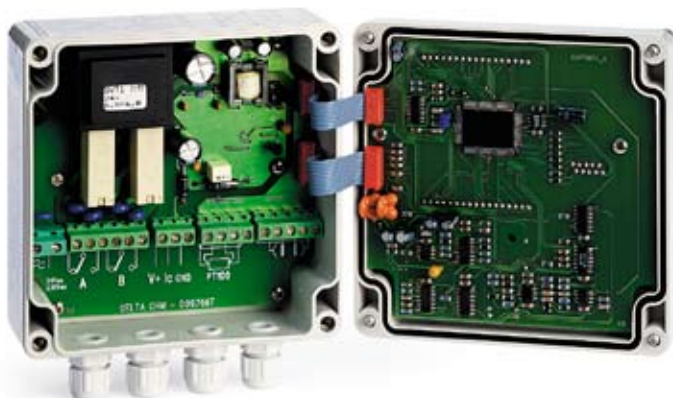

Manual temperature setting

If the temperature probe is not connected or if the probe is broken the measuring unit °C or °F flashes. In this case it is possible to set the temperature compensation value manually.

- Press the CAL key and the °C/°F key together; the message CAL appears at the bottom of the display.
- Using the ▲ and ▼ keys, set the temperature value corresponding to the temperature of the liquid in which you wish to measure conductivity.
- Press CAL to confirm this value. The message CAL disappears.

Calibration of the DO 9786T-R1 / DO 9766T-R1 with conductivity probes

Calibration of the DO 9786T-R1 / DO 9766T-R1 transmitters with conductivity probes:

- Immerse the probe in the buffer solution used for calibration.
- Press the CAL key and the X key together; the message CAL appears at the top of the display.
- The instrument can automatically recognize two standard calibration solutions: a 0.1 molar solution of KCl and a 0.01 molar solution of KCl. The instrument proposes the conductivity value as a function of the measured temperature if the temperature probe is connected, or the manually set temperature.
- Using the ▲ and ▼ keys, adjust the conductivity value measured as a function of the liquid temperature.
- Press CAL to confirm this value. The message CAL disappears.

NOTE: If you want to quit without storing the new calibration, press the °C/°F key.

N.B.: Before calibrating the probe set a cell constant close to the cell constant of the probe that you wish to calibrate with key PRG, function P2. If the message E1 appears during calibration, the instrument is indicating that the probe gain is too high; quit programming (°C/°F button) and increase the value of the cell constant. Likewise, if E2 appears, the instrument is indicating that the probe gain is too low; quit calibration and decrease the cell constant. Repeat the calibration operation.

Programming the parameters

- P1 Temperature coefficient. May be set between 0 and 4.0%/°C (0 and 2.2%/°C).
- P2 Cell constant. May be set between 0.01 and 199.9.
- P3 Conductivity value corresponding to 4 mA at output. May be set between 0 and 199.9 mS.
- P4 Conductivity value corresponding to 20 mA at output. May be set between 0 and 199.9 mS.
- P5 Delay time in the intervention of relay A. May be set between 0 and 250 seconds.
- P6 Delay time in the intervention of relay B. May be set between 0 and 250 seconds.
- P7 Reference temperature of the conductivity measurement. May be set between the values 20.0 or 25.0°C.
- P8 Calibration of Pt100 probe and calibration of analog output in current (see Pt100 probe calibration and analog output calibration).

To change one of these parameters (except P8) press key PRG until the message corresponding to the parameter to be changed appears on the screen. Using the ▲ and ▼ keys, bring the parameter displayed to the desired value. Press OK to confirm.

Pt100 probe calibration

- Connect the Pt100 probe to the instrument. Press the PRG key until the message P8 appears on the display.
- Press the CAL key; the message CAL appears at the bottom of the display and the temperature is shown at the top.
- Immerse the Pt100 probe and a precision thermometer for reference in the zero calibration bath. Wait long enough for the reading to become stable.
- Using the ▲ and ▼ keys, adjust the value of the temperature measured by the Pt100 probe so that it corresponds with the value on the reference thermometer.
- Immerse the Pt100 probe and a precision thermometer in the full scale calibration bath. Wait long enough for the reading to become stable.
- Using the ▲ and ▼ keys, adjust the value of the temperature measured by the Pt100 probe so that it corresponds with the value on the reference thermometer.
- Press OK to confirm.

N.B.: If the temperature shown by the instrument is between +12°C, the instrument calibrates the probe offset, otherwise it calibrates the gain.

Calibrating the analog output

- Press the PRG key until the message P8 appears on the display.
- Connect a precision milliammeter to the analog output.
- Press the **CAL key twice**; the message CAL appears at the top of the display and the message 4.0 at the bottom, indicating calibration at 4 mA.
- Using the ▲ and ▼ keys, adjust the value of the output current so as to have an indication of 4,000 mA on the precision milliammeter.
- Press the CAL key; the message CAL appears at the top of the display and the message 20.0 at the bottom, indicating calibration at 20 mA.
- Using the ▲ and ▼ keys, adjust the value of the output current so as to have an indication of 20,000 mA on the precision milliammeter.
- Press OK to confirm.

Display

Symbol	Description
°C	indicates that the value shown is in °C.
°F	indicates that the value shown is in °F.
µS	indicates that the unit of the value shown is micro Siemens.
mS	indicates that the unit of the value shown is milli Siemens.
A	indicates that the relay A is in closed status.
B	indicates that the relay B is in closed status.

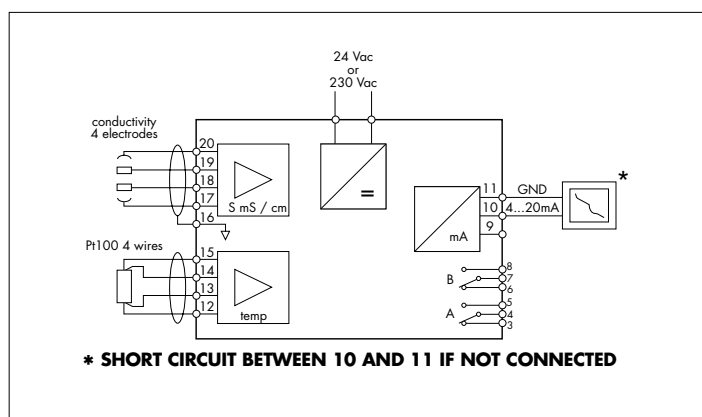


Fig.1 Active transmitter.

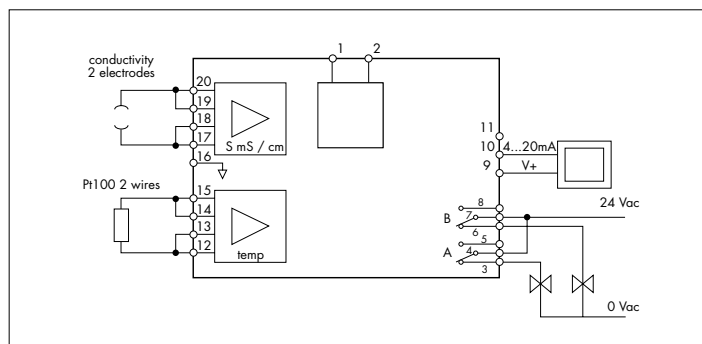


Fig.2 Passive transmitter.


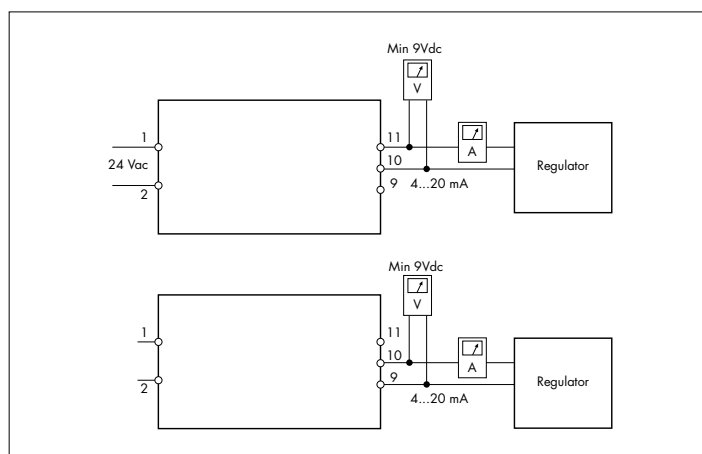


Fig.3 Calibration analog output.

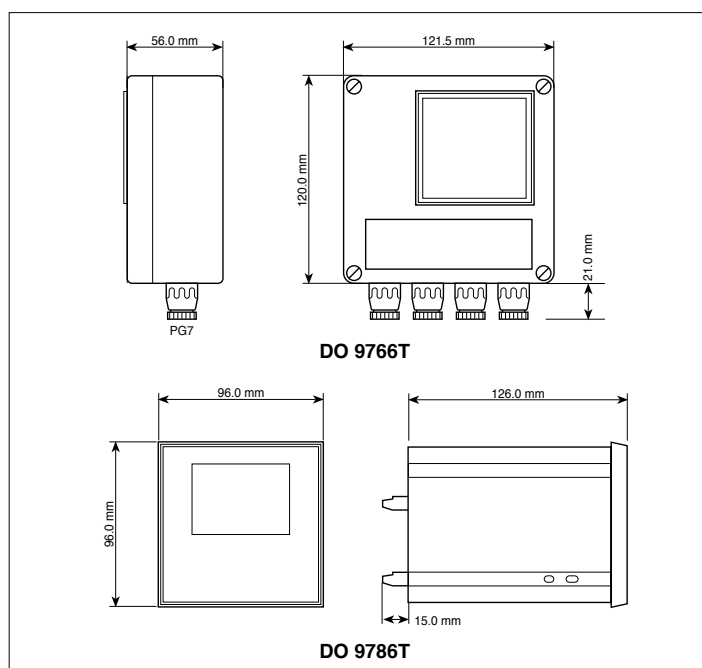

Dimensions

- ON** indicates that the value shown corresponds to the closing thresholds of the contacts of relay A or B.
- OFF** indicates that the value shown corresponds to the opening thresholds of the contacts of relay A or B.

Error signals

- OFL** - Warning which appears during measurement when the value to be displayed is out of scale.
- E1** - Error warning which appears during conductivity calibration to indicate that the probe gain is too high. Press P2 to increase the cell constant value.
- E2** - Error warning which appears during conductivity calibration to indicate that the probe gain is too low. Press P2 to decrease the cell constant value.
- E3** - Error warning which appears to indicate that the instrument is unable to recognize the buffer solution used for automatic calibration. Press the ▲ or ▼ key to make this indication disappear.
- E4** - Reading error on the EEPROM.

APPENDIX

Table of compatibility between range and sensor

Conductivity Range	Nominal cell constant			
	0.01÷0.2	0.2÷2	2÷20	20÷199.9
0÷19.99 µS	✓			
0÷199.9 µS	✓	✓		
0÷1999 µS	✓	✓	✓	
0÷199.9 mS	✓	✓	✓	✓
0÷19.99 mS			✓	✓
0÷1999 mS				✓

Temperature sensor

Temperature	Pt100	Temperature	Pt100
-50°C	80.25 Ω	100°C	138.50 Ω
-25°C	90.15 Ω	125°C	147.94 Ω
0°C	100.00 Ω	150°C	157.32 Ω
25°C	109.73 Ω	175°C	166.62 Ω
50°C	119.40 Ω	199°C	175.47 Ω
75°C	128.98 Ω		

Calculating the temperature coefficient of a solution

If the temperature coefficient of the solution is not known, it may be determined using the DO 9786T/DO 9766T.

- Set the temperature coefficient at 0.0%/°C (parameter P1).
- The following measurements should be taken as close as possible to the work point, between 5°C and 70°C, for greater accuracy.
- Immerse the probe in the testing liquid. Wait for the measurement to become stable.
- Take note of the temperature and of the conductivity.
- Increase the solution temperature by at least 10°C.
- Take note of the temperature and of the conductivity.
- Calculate the temperature coefficient using the following formula:

$$\alpha = \frac{(G_x - G_y) \times 100\%}{G_y(T_x - 20) - G_x(T_y - 20)} \quad (\text{reference temperature } 20^\circ\text{C})$$

Where:

G_x conductivity at temperature T_x
G_y conductivity at temperature T_y

N.B.: if the reference temperature is 25°C, replace 20 with 25.

- Set the temperature coefficient with the value calculated as above (parameter P1).

Calibration of the instrument for measuring conductivity

The conductivity measurement depends strongly on the temperature of the liquid that is to be measured; this relationship must be considered during calibration.

Calibration of the instrument alone by means of a precision resistance

This is a sure and accurate method for calibrating the instrument alone, but it does not allow for the variations of the cell constant that may occur, nor of the state of efficiency and cleanliness of the cell.

The precision resistance used for calibration will be chosen according to the scale that you want to calibrate. Typical values are the following:

Conductivity	Resistance
100,0 µS	10.000 Ω
500,0 µS	2.000 Ω
1000 µS	1.000 Ω
5000 µS	200 Ω
10,00 mS	100 Ω
50,00 mS	20 Ω
100,0 mS	10 Ω
500,0 mS	2 Ω
1000 mS	1 Ω

The precision resistance will be connected to the end of the cable that connects the probe to

the instrument. This ensures greater accuracy of calibration. Disable the temperature compensation α_T during the calibration of the instrument with the precision resistances.

Calibration with standard solutions

In this case too, for the calibration of the instrument, cable and measuring probes in a standard solution, the greatest attention must be paid to the temperature of the solutions and the cleanliness of the measuring cell. It is advised not to carry out calibration below 500 µS/cm. Solutions with low conductivity must be kept closed in their containers. Contact with the air increases their value due to the absorption of CO₂.

The regulations for the preparation of standard solutions with a base of KCl dissolved in water with a high degree of purity supply the method and percentages of KCl and water to be mixed.

DELTA OHM supplies four solutions for calibration:

HD8747: Standard calibration solution 0.001 mol/l equal to 147 µS/cm @25°C, 200cc.

HD8714: Standard calibration solution 0.01 mol/l equal to 1413 µS/cm @25°C, 200cc.

HD8712: Standard calibration solution 0.1 mol/l equal to 12880 µS/cm @25°C, 200cc.

HD87111: Standard calibration solution 1 mol/l equal to 111800 µS/cm @25°C, 200cc.

Care and maintenance of the conductivity cell

In conductivity measurement systems in industrial plants, if the installation is correctly made, readings are generally reliable for a long time. The important thing is to carry out correct, programmed maintenance of the measuring cell.

Abrasion of the cable due to continued swinging movements must be avoided, as must the formation of deposits and scale on the cell which can change its geometrical structure.

The cell must always be immersed in the liquid that is to be measured. In the industrial field, measurements may range from highly pure water to sewage or water contaminated by corrosive substances.

It is good practice to check the compatibility of the materials of which the cell and the connecting cable are made with the liquid in which the measurement is to be taken. Check that there are no floating bodies, suspended granules that may be more or less conductive, or which could get stuck inside the cell, thus leading to incorrect measurements.

To clean the cell use detergents or substances suitable for the material of which the cell is made.

Selecting the cell constant and installation

The measurement range of the liquid to be examined determines the choice of the cell constant to be used.

Installation of the cell will vary according to the application. On the whole, the following points must be considered:

- Choose the correct cell and cell constant, suitable for the application.
- Use suitable materials, cable, cell, supports, so as to resist corrosion and the influence of atmospheric agents.
- The sensor/cell must be firmly fixed, in a place where they are easily accessible for maintenance.
- The liquid in which the sensor is immersed must be a representative part of the whole that is to be measured.
- There must be a moderate flow of liquid so that an updated sample of liquid arrives at the electrodes. Excessive movement or flow causes turbulence and air bubbles between the electrodes. As an air bubble is not conductive, it modifies the volume of the cell and changes the constant.
- Install the sensor in such a way that sludge or particles of material cannot be deposited inside it.
- If installed in containers where high currents are circulating, the conductivity cell may present measuring problems.
- The maintenance and cleaning interval depends on the quality of the liquid in which the cell is installed.

Order code

DO 9786T: Conductivity transmitter 4÷20 mA passive or active, power supply 24 Vac with double display 96x96 mm, for panel mounting.

DO 9766T: Conductivity transmitter 4÷20 mA passive or active, power supply 24 Vac with double display 122x120 mm, for use on the field.

SPT 86: Combined industrial conductivity and temperature probe in POCAN with 4 platinum electrodes, cell constant K = 0.7, 1.5 meters cable, Pt100 with 2 wires. Temperature 0÷90°C.

SPTKI 10: Combined industrial conductivity probe in Glass with 2 black oxidized platinum electrodes, cell constant K = 1, S7/PG13 screw-joint, 2 wires output: eurostandard S7. Temperature 0÷100°C.

SPTKI 11: Combined industrial conductivity and temperature probe in Rytron with 2 graphite electrodes, cell constant K = 1, 5 meters cable, Pt100 with four wires. Temperature 0÷50°C.

SPTKI 12: Combined industrial conductivity and temperature probe in Rytron with 2 platinum electrodes, cell constant K = 01, 5 meters cable, Pt100 with four wires. Temperature 0÷50°C.

SPTKI 13: Combined industrial conductivity and temperature probe in Rytron with 2 platinum electrodes, cell constant K = 10, 5 meters cable, Pt100 with four wires. Temperature 0÷50°C.

HD 882 M100/300: Temperature probe with Pt100 sensor, miniature head, shaft Ø6x300 mm.

HD 882 M100/600: Temperature probe with Pt100 sensor, miniature head, shaft Ø6x600 mm.


HD 8747: Calibration solution 0.001 mol/l corresponding to 147 µS/cm at 25°C, 200cc.

HD 8712: Calibration solution 0.1 mol/l corresponding to 12,880 µS/cm at 25°C, 200cc.


HD 8714: Calibration solution 0.01 mol/l corresponding to 1413 µS/cm at 25°C, 200cc.

HD 87111: Calibration solution 1 mol/l corresponding to 111800 µS/cm at 25°C, 200cc.


SPT 400.001
cell constant K=0.01

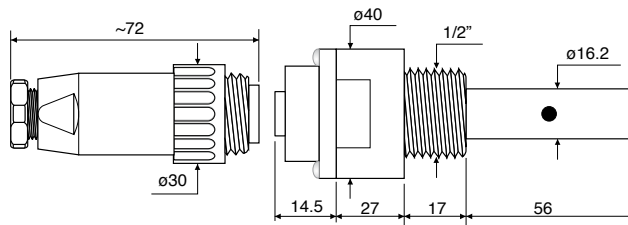


SPT 86
cell constant K=0.7

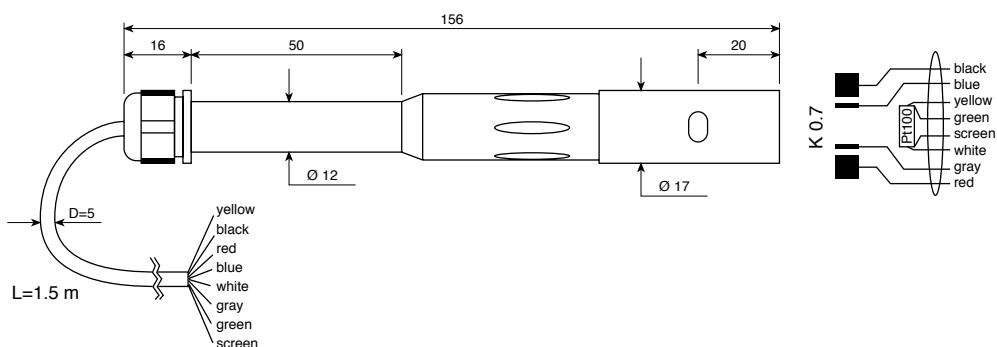


SPTKI 10
cell constant K=1

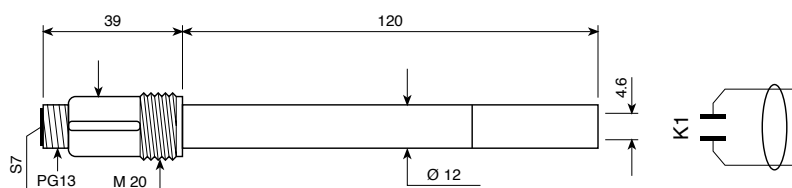


SPTKI 11
cell constant K=1

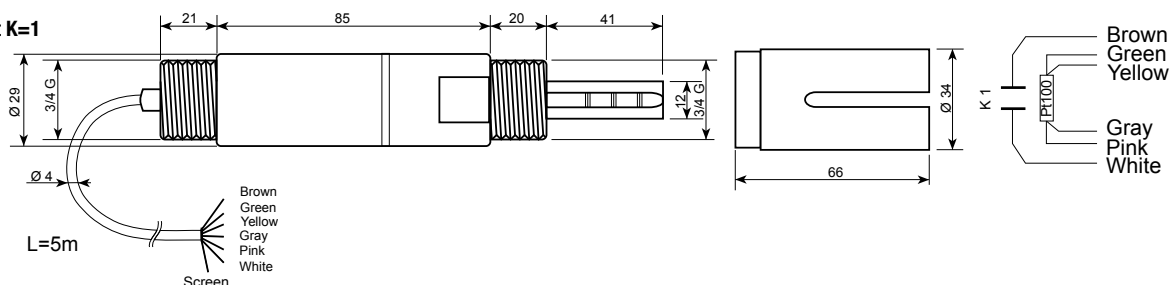

SPTKI 12
cell constant K=0.1

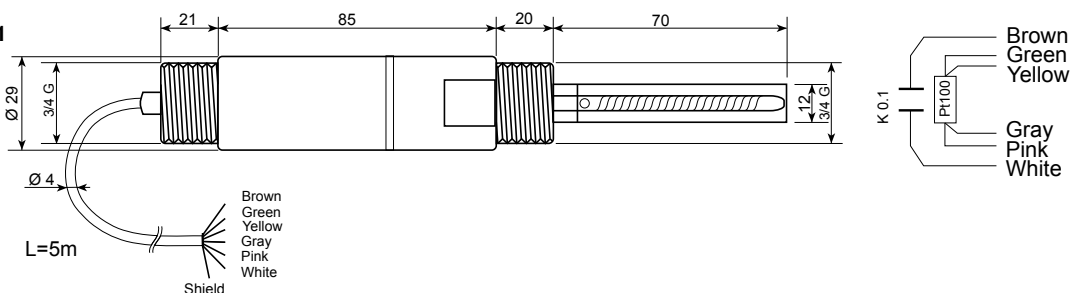

SPTKI 13
cell constant K=10

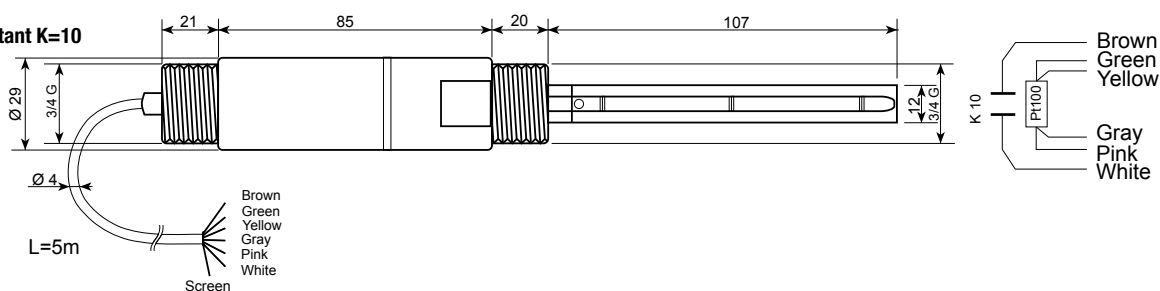

	Cell constant	Measuring range	Temperature range	Material	Electrodes	Temperature sensor	Max. pressure	Connection
SPT 400.001	K=0.01	0.05÷19.9µS	0÷120°C	AISI 316 - PTFE	2 AISI 316	-	12bar	4-pole connector
SPT 86	K=0.7	5µS÷20mS	0÷90°C	Pocan	4 platinum	Pt100 2 wire	6bar	1.5 m cable
SPTKI 10	K=1	100µS÷200mS	0÷100°C	Glass	2 platinum	-	6bar	S7
SPTKI 11	K=1	100µS÷10mS	0÷50°C	Ryton	2 platinum	Pt100 4 wire	6bar	5 m cable
SPTKI 12	K=01	1µS÷1mS	0÷50°C	Ryton	2 platinum	Pt100 4 wire	6bar	5 m cable
SPTKI 13	K=10	10µS÷200mS	0÷50°C	Ryton	2 platinum	Pt100 4 wire	6bar	5 m cable



HD 2109.1, HD 2109.2 DISSOLVED OXYGEN - TEMPERATURE METERS

The **HD2109.1** and **HD2109.2** are portable instruments with a large LCD display. They measure the concentration (in mg/l) of dissolved Oxygen in liquids, the saturation index (in %) and the temperature using SICRAM combined probes of polarographic type with two or three electrodes and integrated temperature sensor. Temperature only is measured by Pt100-SICRAM or direct 4 wire-immersion, penetration or contact probes. Thanks to an internal pressure sensor, the instruments automatically compensate for barometric pressure. The instrument anticipates automatic compensation of the Oxygen probe membrane permeability and of the salinity of the liquid being examined. The dissolved Oxygen probe's quick calibration function guarantees timely correctness of the performed measurements. The dissolved Oxygen and the temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside. The HD2109.2 is a **datalogger**. It stores up to 18,000 dissolved Oxygen concentration, saturation index measurements, barometric pressure and temperature samples which can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing interval, printing, and baud rate can be configured using the menu. The HD2109.1 and HD2109.2 models are fitted with an RS232C serial port and can transfer to a PC the acquired measurements or to a portable printer in real time. The *Max*, *Min* and *Avg* function calculates the maximum, minimum or average values. Other functions include: the relative measurement REL, the Auto-HOLD function, and the automatic turning off which can also be excluded.

The instruments have IP67 protection degree.



INSTRUMENT TECHNICAL CHARACTERISTICS

Measured quantities: mg/l O₂, sat. % O₂, mbar, °C, °F

Instrument

Dimensions (Length x Width x Height)	185x90x40mm
Weight	470g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ digits plus symbols Visible area: 52x42mm

Operating conditions

Working temperature	-5...50°C
Storage temperature	-25...65°C
Working relative humidity	0...90%RH without condensation
Protection degree	IP67

Power

Batteries	4 1.5V type AA batteries
Autonomy	200 hours with 1800mAh alkaline batteries
Power absorbed with instrument off	20µA
With dissolved oxygen probe	40µA
Mains (SWD10)	Output mains adapter 12Vdc / 1A

Security of memorized data

Unlimited, independent of battery charge conditions

Time

Date and time	Schedule in real time
Accuracy	1min/month max error

Measured values storage - model HD2109.2

Type	2000 pages containing 9 samples each
Quantity	18,000 samples composed of 4 parameters: mg/l O ₂ - %O ₂ - mbar - (°C or °F)
Selectable storage interval	1s, 5s, 10s, 15s, 30s, 60s (1min), 120s (2min), 300s (5min), 600s (10min), 900s (15min), 1200s (20min), 1800s (30min) and 3600s (1hour)

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
selectable print interval immediate	1s, 5s, 10s, 15s, 30s, 60s (1min), 120s (2min), 300s (5min), 600s (10min), 900s (15min), 1200s (20min), 1800s (30min) and 3600s (1hour)

USB interface - model HD2109.2

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Connections

Input for Oxygen and temperature probes	8-pole male DIN45326 connector
Serial and USB interface	8-pole MiniDin connector
Mains adapter	2-pole connector (positive at centre)

Measurement of the concentration of dissolved Oxygen

Measurement range	0.00...90.00mg/l
Resolution	0.01mg/l
Accuracy (60...110%, 1013mbar, 20...25°C)	±0.03mg/l±1digit



HD40.1



SWD10

Measurement of the saturation index of dissolved Oxygen

Measurement range	0.0...600.0‰
Resolution	0.1‰
Accuracy	±0.3% ±1digit (in the range 0.0...199.9%) ±1% ±1digit (in the range 200.0...600.0%)

Measurement of barometric pressure

Measurement range	0.0...1100.0mbar
Resolution	0.1mbar
Accuracy	±2mbar±1digit between 18 and 25°C ±(2mbar+0.1mbar/°C) in the remaining range

Setting the salinity

Setting range	0.0...70.0mg/l
Resolution	0.1mg/l

Temperature measurement with the sensor inside the dissolved Oxygen probe

Measurement range	0...+45°C
Resolution	0.1°C
Accuracy	±0.1°C
Drift after 1 year	0.1°C/year

Temperature measurement by Instrument with Pt100 probe

Pt100 measurement range	-200...+650°C
Resolution	0.1°C
Accuracy	±0.21°C
Drift after 1 year	0.1°C/year
Automatic temperature compensation	0...50°C

TECHNICAL DATA OF PROBES AND MODULES EQUIPPED WITH INSTRUMENT Temperature probes Pt100 sensor using SICRAM module

Model	Type	Working range	Accuracy
TP87	Immersion	-50°C...+200°C	±0.25°C (-50°C...+200°C)
TP472I	Immersion	-196°C...+500°C	±0.25°C (-196°C...+350°C) ±0.4°C (+350°C...+500°C)
TP472I.0	Immersion	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP473P.0	Penetration	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP474C.0	Contact	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP472I.5	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP472I.10	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)

Temperature drift @20°C 0.003%/°C


Direct 4 wire Pt100 probes

Model	Type	Working range	Accuracy
TP47.100	4 wire Pt100	-50...+400°C	Class A

Temperature drift @20°C 0.003%/°C

Oxygen probe – dimensions and characteristics

Model	D09709SS	D09709SS.5
Type	Polarographic probe, Silver anode, Platinum cathode	
Application range		
Oxygen concentration	0.00...60.00mg/l	
Functioning temperature	0...45°C	
Accuracy instrument with probe	1% FS	
Membrane	Replaceable	
Cable length	2m	5m

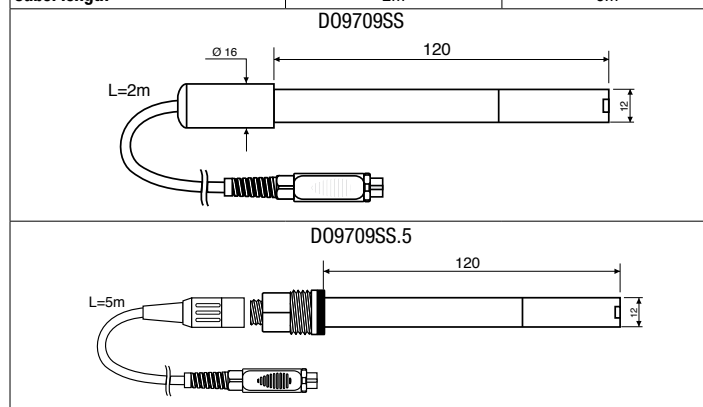

ORDER CODES

HD2109.1: The kit is composed of: instrument HD2109.1, calibrator D09709/20, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software.

The probes and data transfer cable must be ordered separately.

HD2109.2: The kit is composed of: instrument HD2109.2 **datalogger**, calibrator D09709/20, connection cable for serial output **HD2101/USB**, 4 1.5V alkaline batteries, operating manual, case and DeltaLog9 software.

The probes and data transfer cable must be ordered separately.

HD2110CSNM: 8-pole connection cable MiniDin - Sub D 9-pole female for RS232C.

C.206: Serial connection cable with USB connector for PC and 8-pole MiniDin male connector for the instrument

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole MiniDin (not suitable for HD2109.1K).

DeltaLog9: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply 100-240 Vac/12Vdc-1A mains voltage

HD40.1: 24-column portable thermal printer, serial interface, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm in diameter.

BAT-40: Spare battery pack for HD40.1 printer with built-in temperature sensor.

HD22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by bench-top meters of the series HD22...with cable HD22.2.1 (**optional**) or power supplier SWD10 (**optional**).

HD22.3: Laboratory electrode holder composed of base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.

Solutions

D09700: zero solution.

D09701: electrolyte solution.

Combined dissolved Oxygen/temperature probes

D09709 SS: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 2m. Ø12mm x 120mm.

D09709 SS.5: The kit includes: combined probe for measurement of O₂ and temperature, replaceable membrane, Ø 12mm x Ø 12mm. Cable length 5m, three membranes, 50ml of zero solution, 50ml of electrolyte solution.

Temperature probes complete with SICRAM module

TP87: Pt100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP472I.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP472I.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP472I.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes without SICRAM module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes



D09700

D09701



HD 98569 MULTIPARAMETER INSTRUMENT: pH - CONDUCTIVITY DISSOLVED OXYGEN - TEMPERATURE

The **HD 98569** is a portable multi-parameter data logger for electrochemical measures: **pH**, **conductivity**, **dissolved oxygen** and **temperature**. It is fitted with a large back-lighted LCD display.

The instrument measures:

- **pH, mV, redox potential (ORP)** with pH, redox or combined pH/temperature electrodes **complete with SICRAM module**;
- **conductivity, resistivity** in liquids, **total dissolved solids (TDS)**, and **salinity** with combined 4-ring and 2-ring conductivity and temperature probes **with SICRAM module**.
- **Concentration of dissolved oxygen** in liquids (in mg/l), **saturation index** (in %) **using SICRAM combined probes** of polarographic type with two or three electrodes and integrated temperature sensor.

The instrument is fitted with input for the measurement of **temperature** with Pt100 immersion, penetration or contact probes with SICRAM module.

- The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 8 buffers. Temperature compensation can be automatic or manual.
- The conductivity probe calibration can be performed with automatically detected conductivity calibration solutions: 147µS/cm, 1413µS/cm, 12880µS/cm, 111800µS/cm or manually with calibration solutions having different values.
- The dissolved oxygen probe's quick calibration function guarantees long-term correctness of the performed measurements.
- pH, conductivity dissolved oxygen and temperature probes fitted with SICRAM module can store factory and calibration data inside.

The HD 98569 is a **data logger**, it stores up to 200 single screens (labels) and up to 9000 samples in continuous storage mode: pH or mV, conductivity or resistivity or TDS or salinity, concentration of dissolved oxygen and saturation index and temperature.

The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0-1.1.

The instruments equipped with **HD22BT** Bluetooth option can transfer the data without any connection to a PC fitted with USB/Bluetooth converter HD USBK1, or to the printer **HD40.2** with Bluetooth interface or to a PC with Bluetooth input.

The serial connection RS232C can be used for direct printing of labels with a 24 column printer (**HD40.1** or **HD40.2**).

The software **DeltaLog11** (vers. 2.0 and subsequent ones) allows instrument management and configuration, and data processing on PC.

Technical characteristics of HD 98569

Measured values

pH - mV
 χ - Ω - TDS - NaCl
 mg/l O₂ - %O₂
 °C - °F

Instrument

Dimensions

(Length x Width x Height)

250x100x50mm

Weight

640g (complete with batteries)

Materials

ABS, rubber

Display

Graphic, back lighted LCD, 56x38mm.
 128x64 points

Operating conditions

Working temperature

-5 ... 50°C

Storage temperature

-25 ... 65°C

Working relative humidity

0 ... 90% RH without condensate

Protection degree

IP66

Power

Batteries

4 batteries 1.5V type AA

Autonomy (with probes connected)

25 hours with 1800mAh alkaline batteries

Mains (cod. SWD10)

12Vdc/1A (positive at centre)

Security of memorized data

Unlimited

Time

Date and hour

Schedule in real time

Accuracy

1min/month max. departure

Continuous storage (LOG key)

Quantity

9000 samples of the three inputs

Type

organised in 1800 pages containing 5 samples each

Storage interval

1s ... 999s

Storage on command (MEM key)

Quantity

200 samples of the three inputs

Type

organised in 200 pages containing 1 sample each



① Only conductivity probes with SICRAM module.

② Input for O₂ and temperature probes or for only temperature probes with SICRAM module.

③ Input for pH, mV, pH and temperature probes or for only temperature probes with SICRAM module.

④ External Power supply.

⑤ RS232 or USB interface.

Calibration storage	
pH and Dissolved Oxygen	Last 8 pH and dissolved oxygen calibrations. The last 2 are saved in the SICRAM memory of the probe as well.
Conductivity	Last calibration is saved in the SICRAM memory of the probe.
RS232C serial interface	
Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow control	Xon/Xoff
Length of serial cable	Max 15m
USB interface	
Typ	1.1 - 2.0 electrically isolated

Bluetooth interface	
	Optional for PCs fitted with Bluetooth input or HD USB. KL1 Bluetooth / RS232 adapter. The interface can be installed in Delta Ohm only.

Connections	
Enabled inputs for temperature probes with SICRAM module	pH/mV and O ₂ inputs.

Input for pH/temperature with SICRAM module	8-pole male DIN45326 connector
---	--------------------------------

Input for conductivity/temperature with SICRAM module	8-pole male DIN45326 connector
---	--------------------------------

Input for dissolved oxygen/temperature with SICRAM module	8-pole male DIN45326 connector
---	--------------------------------

RS232C / USB interface	8-pole MiniDin female connector
------------------------	---------------------------------

Bluetooth	Optional
-----------	----------

Mains adapter	2-pole(Ø5.5mm- Ø2.1mm). Positive at centre (e.g. SWD10).
---------------	--

■ Measurement of pH by instrument

Measuring range	-9.999...+19.999pH
Resolution	0.01 o 0.001pH selectable from menu
Accuracy	±0.001pH ±1digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	Offset1 > 20mV Slope > 63mV/pH or Slope < 50mV/pH Sensitivity > 106.5% or Sensitivity < 85%
Calibration points	Up to 5 points from a list of 8 automatically detected buffers
Temperature compensation	-50...150°C
Automatically detected standard solutions @25°C	1.679pH - 4.000pH - 4.010pH 6.860pH - 7.000pH - 7.648pH 9.180pH - 10.010pH

Measurement of mV by instrument

Measuring range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	±0.1mV ±1digit
Drift after 1 year	0.5mV/year

■ Measurement of conductivity by instrument

Measurement range (K cell=0.01)	0.000...1.999μS/cm	Resolution 0.001μS/cm
Measurement range (K cell=0.1)	0.00...19.99μS/cm	0.01μS/cm
Measurement range (K cell=1)	0.0...199.9μS/cm	0.1μS/cm
	200...1999μS/cm	1μS/cm
	2.00...19.99mS/cm	0.01mS/cm
	20.0...199.9mS/cm	0.1mS/cm
Measurement range (K cell=10)	200...1999mS/cm	1mS/cm
Accuracy (conductivity) instrument	±0.5% ±1digit	

Measurement of resistivity by instrument

Measurement range (K cell=0.01)	Up to 1GΩ·cm	Resolution (*) 0.1Ω·cm 1Ω·cm 0.01kΩ·cm 0.1kΩ·cm 1kΩ·cm 1MΩ·cm 0.1Ω·cm
Measurement range (K cell=0.1)	Up to 100MΩ·cm	
Measurement range (K cell=1)	5.0...199.9Ω·cm	
	200...999Ω·cm	
	1.00k...19.99kΩ·cm	
	20.0k...99.9kΩ·cm	
	100k...999kΩ·cm	
	1...10MΩ·cm	
Measurement range (K cell=10)	0.5...5.0Ω·cm	
Accuracy (resistivity) instrument	±0.5% ±1digit	

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity (μS/cm)	Resistivity (MΩ·cm)	Conductivity (μS/cm)	Resistivity (MΩ·cm)
0.001 μS/cm	1000 MΩ·cm	0.01 μS/cm	100 MΩ·cm
0.002 μS/cm	500 MΩ·cm	0.02 μS/cm	50 MΩ·cm
0.003 μS/cm	333 MΩ·cm	0.03 μS/cm	33 MΩ·cm
0.004 μS/cm	250 MΩ·cm	0.04 μS/cm	25 MΩ·cm
...

Measurement of total dissolved solids Resolution

(with coefficient χ /TDS=0.5)		
Measurement range (K cell=0.01)	0.00...1.999mg/l	0.005mg/l
Measurement range (K cell=0.1)	0.00...19.99mg/l	0.05mg/l
Measurement range (K cell=1)	0.0...199.9 mg/l	0.5 mg/l
	200...1999 mg/l	1 mg/l
	2.00...19.99 g/l	0.01 g/l
	20.0...199.9 g/l	0.1 g/l
	100...999 g/l	1 g/l
Measurement range (K cell=10)		
Accuracy (total dissolved solids) instrument	±0.5% ±1digit	

Measurement of salinity

Measurement range	0.000...1.999g/l	Resolution 1mg/l 10mg/l 0.1 g/l
	2.00...19.99g/l	
	20.0...199.9 g/l	
Accuracy (salinity) instrument	±0.5% ±1digit	

Automatic/manual temperature compensation

0...100°C with $\alpha_T = 0.00...4.00\%/^{\circ}\text{C}$

Reference temperature

0...50°C (Default values 20°C or 25°C)

Conversion factor χ / TDS

0.4...0.8

Admitted cell constants K (cm⁻¹)

0.01...20.00

Automatically detected standard solutions (@25°C)

147μS/cm
1413μS/cm
12880μS/cm
111800μS/cm

■ Measurement of concentration of dissolved oxygen

Measurement range	0.00...90.00mg/l
Resolution	0.01mg/l
Accuracy instrument	$\pm 0.03\text{mg/l} \pm 1\text{digit}$ (60...110%, 1013mbar, 20...25°C)

Measurement of saturation index of dissolved oxygen

Measurement range	0.0...600.0%
Resolution	0.1%
Accuracy instrument	$\pm 0.3\% \pm 1\text{digit}$ (in the range 0.0...199.9%) $\pm 1\% \pm 1\text{digit}$ (in the range 200.0...600.0%)

Salinity setting

Setting	directly from menu or automatically by conductivity measurement
Setting range	0.0...70.0g/l
Resolution	0.1g/l

Temperature measurement with the sensor inside the O_2 probe

Measurement range	0.0...50.0°C
Resolution	0.1°C
Accuracy instrument	$\pm 0.1^\circ\text{C}$
Drift after 1 year	0.1°C/year
Automatic temperature compensation	0...50°C

■ Measurement of temperature by instrument

Pt100 Measurement range	-50...+150°C
Resolution	0.1°C
Accuracy instrument	$\pm 0.1^\circ\text{C} \pm 1\text{digit}$
Drift after 1 year	0.1°C/year

24 column printing example

```

HD 98569
pH / chi / Oxy / temperature
Ser num=12345678

2007 - 01 - 31 12:00:00

LAB POSITION #1

Operator = Amministratore

SAMPLE ID = 00000001

pH EL sernum = 01234567
pH = 7.010
pH out of calibration !

O2 EL sernum = 76543210
mg/l O2 = 5.59

chi EL sernum = 98756410
mS = 2.177

Temp = 25.0°C ATC
    
```

Ordering codes

HD 98569: The kit is composed of: instrument **data logger** HD 98569 for measurement of pH - redox - conductivity - resistivity - TDS - salinity - concentration of dissolved oxygen - saturation index - temperature, 4 1.5V batteries type AA, instructions manual, software DeltaLog11 (vers. 2.0 and subsequent ones), carrying case and SICRAM module KP471.1 (cable 1 meter).

The pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for data download to PC or printer have to be ordered separately.

HD2110CSNM: 8-pole connection cable Mini Din - Sub D 9-pole female for RS232C, for connection to PC with RS232C USB input.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole Mini Din for connection to PC with USB input.

DeltaLog11: Further unit of software (vers. 2.0 and subsequent ones) for data download and management on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.

HD40.1: 24-column portable thermal printer, serial interface, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

HD40.2: 24-column portable thermal printer, **Bluetooth and serial interface**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (**optional**) or the cable HD 2110 CSNM (**optional**).

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm in diameter.

BAT-40: Spare battery pack for HD40.1 printer with built-in temperature sensor.

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. For Ø12mm electrodes. Powered by bench top meters of series HD22... with cable HD22.2.1 (**optional**) or supplier SWD10 (**optional**)

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

HD22BT: Bluetooth module for wireless data transmission from instrument PC. **The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.**


HD USB.KL1: USB/Bluetooth converter to be connected to the PC for wireless data transmission from the instrument with HD22BT module.

SICRAM Modules with S7 input for pH electrodes

KP471.1: SICRAM module for pH electrodes with S7 standard connection, cable L=1m.


KP471.2: SICRAM module for pH electrodes with S7 standard connection, cable L=2m.

KP471.5: SICRAM module for pH electrodes with S7 standard connection, cable L=5m.

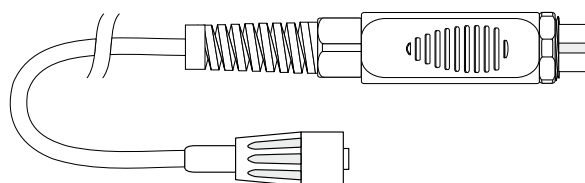


pH Electrodes to be connected to KP471... SICRAM module

KP20: Combined pH electrode for general use, GEL-filled, with screw connector S7, body in Epoxy,

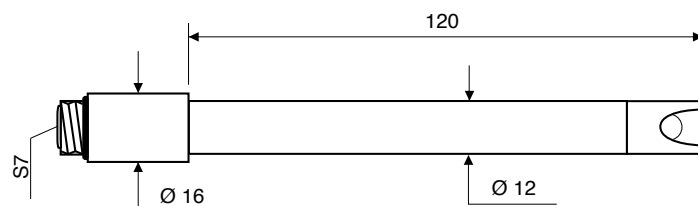


KP 50: Combined pH electrode pH for general use, varnishes, emulsions, GEL-filled, with S7 screw connector, body in glass.

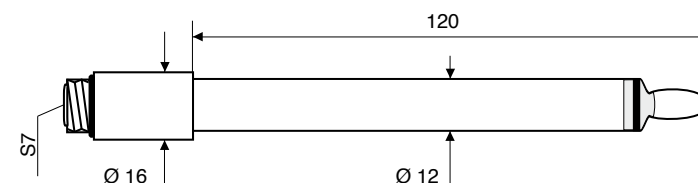


KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. gel-filled, with screw connector S7, body in glass.




KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. GEL-filled, with screw connector S7, body in glass

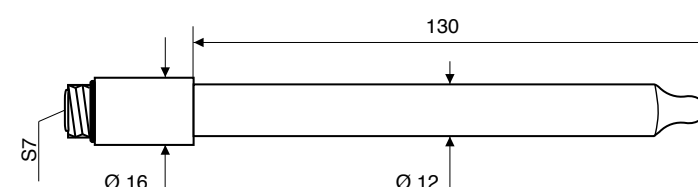

KP 64: Combined pH electrode for water, varnishes, emulsions, etc. reference filling solution KCl 3M, with S7 screw connector, body in glass.

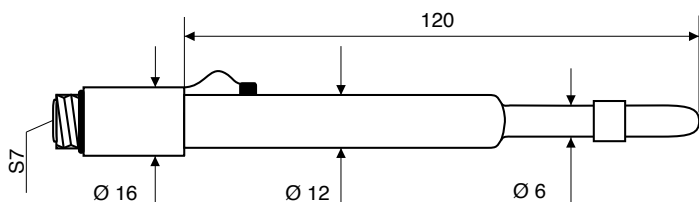

KP 70: Combined pH electrode, micro diam. 6 x L=70mm, GEL-filled, for paste, bread, cheese, etc, with S7 connector, body in glass.

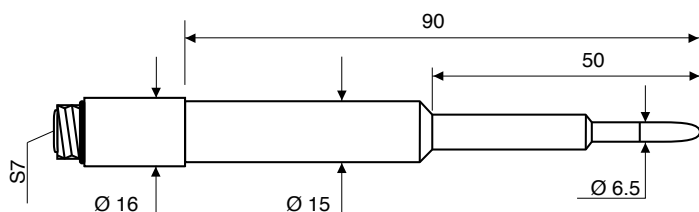

KP 80: Combined pointed pH electrode, gel-filled, with screw connector S7, body in glass.




ORP Electrodes to be connected to KP471... SICRAM module

KP90: REDOX PLATINUM electrode, with screw connector S7, reference filling solution KCl 3M, body in glass.




pH Electrodes with SICRAM module

KP 50TS: Combined pH/temperature electrode, Pt100 sensor, GEL-filled, with SICRAM module, body in glass, general use, varnishes, emulsions. Cable length 1m.

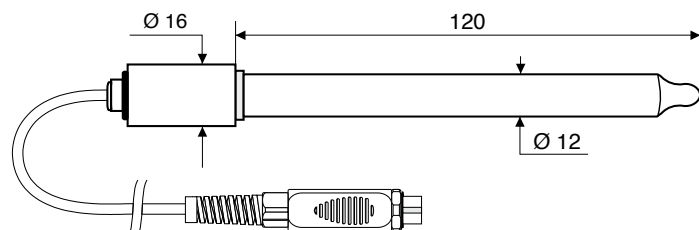

KP63TS: Combined pH/temperature electrode, Pt100 sensor, GEL-filled, with SICRAM module, body in glass, Ag/AgCl sat KCl.

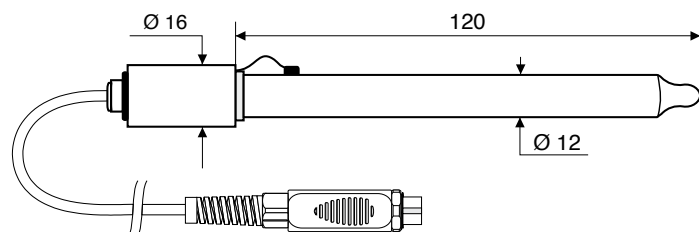

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 500cc.

HDR468: Redox buffer solution 468mV 500cc.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for refilling of electrodes.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 200cc.

HD62PP: Protein cleaning (pepsin in HCl) - 200cc.


HD62RF: Regeneration (fluorhydric acid) - 100cc.

HD62SC: Solution for electrode preservation - 200cc.

Combined conductivity and temperature probes with SICRAM module


SP06TS: Combined conductivity and temperature 4-electrode cell, body in Pocan. Cell constant K=0.7.

Measurement range 5µS/cm ... 200mS/cm, 0...90°C.

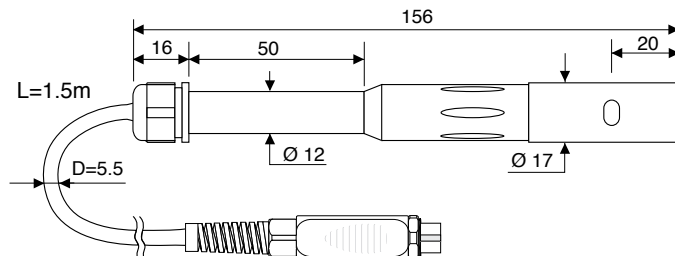


SPT401.001S: Combined conductivity and temperature 2-electrode cell in stainless steel AISI 316. Cell constant K=0.01. Cable 2m.

Measurement range 0.04µS/cm ... 20µS/cm, 0...120°C. Measurement in closed-cell.

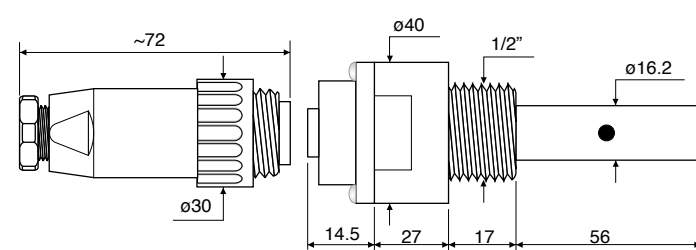


SPT01GS: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K=0.1.

Measurement range 0.1µS/cm ... 500µS/cm, 0...80°C.

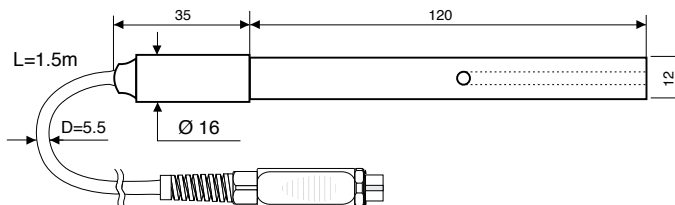


SPT1GS: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K=1.

Measurement range 10µS/cm ... 10mS/cm, 0...80°C.

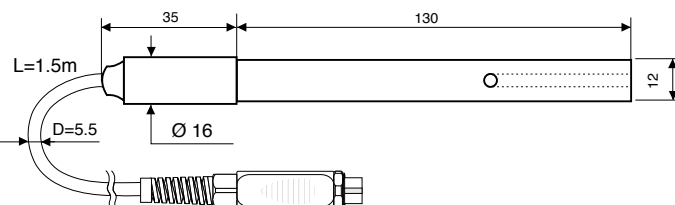

SPT10GS: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K=10.

Measurement range 500µS/cm ... 200mS/cm, 0...80°C.

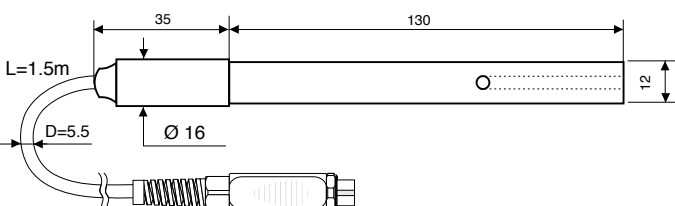

Standard calibration solutions

HD8747: Standard calibration solution 0.001 mol/l equal to $147 \mu\text{S}/\text{cm}$ @ 25°C - 200cc.


HD8714: Standard calibration solution 0.01 mol/l equal to $1413 \mu\text{S}/\text{cm}$ @ 25°C - 200cc.

HD8712: Standard calibration solution 0.1 mol/l equal to $12880 \mu\text{S}/\text{cm}$ @ 25°C - 200cc.


HD87111: Standard calibration solution 1 mol/l equal to $111800 \mu\text{S}/\text{cm}$ @ 25°C - 200cc.

Combined dissolved oxygen/temperature probes

D09709 SS: The kit includes: combined probe for the measurement of O_2 and temperature with replaceable membrane, three membranes totally. 50ml of zero solution, 50ml of electrolyte solution. Cable length 2m. $\varnothing 12\text{mm} \times 120\text{mm}$.

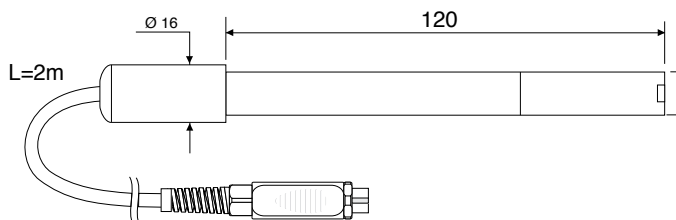

D09709 SS.5: The kit includes: combined probe for the measurement of O_2 and temperature with replaceable membrane, three membranes totally. 50ml of zero solution, 50ml of electrolyte solution. Cable length 5m. $\varnothing 12\text{mm} \times 120\text{mm}$.

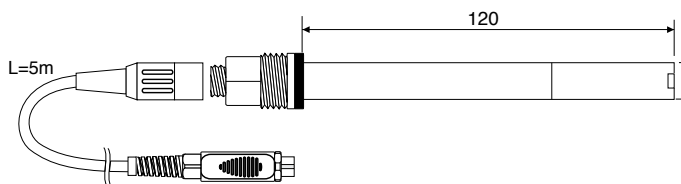

Accessories for combined dissolved oxygen/temperature probes

D09709 SSK: Accessory kit for the D09709 SS probe consisting of three membranes, 50ml of zero solution, 50ml of electrolyte solution.

D09709.20: Calibrator for polarographic probes D09709SS and D09709SS.5.

Temperature probes with SICRAM module

TP87: Pt100 sensor immersion probe. Probe's stem $\varnothing 3\text{mm}$, length 70mm. Cable length 1 metre.

TP4721.0: Pt100 sensor immersion probe. Stem $\varnothing 3\text{mm}$, length 230 mm. Cable length 2 metres.

TP473P.0: Pt100 sensor penetration probe. Stem $\varnothing 4\text{mm}$, length 150 mm. Cable length 2 metres.

TP474C.0: Pt100 sensor contact probe. Stem $\varnothing 4\text{mm}$, length 230mm, contact surface $\varnothing 5\text{mm}$. Cable length 2 metres.

TP475A.0: Pt100 sensor air probe. Stem $\varnothing 4\text{mm}$, length 230mm. Cable length 2 metres.

TP4721.5: Pt100 sensor immersion probe. Stem $\varnothing 6\text{mm}$, length 500 mm. Cable length 2 metres.

TP4721.10: Pt100 sensor immersion probe. Stem $\varnothing 6\text{mm}$, length 1,000mm. Cable length 2 metres.





HD 3405.2 BENCH-TOP pH METER

The **HD3405.2** is a 4 bench top instrument for electrochemical measures: **pH, and temperature**.

The displayed data can be stored (**datalogger**) and can be transferred to PC or serial printer thanks to the multi-standard serial port RS232C and USB2.0 and software DeltaLog9 (Vers.2.0 and subsequent ones). The storing and printing parameters can be set from menu. The **HD3405.2** measures **pH, redox potential (ORP)** in mV. It measures **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The pH electrode calibration can be carried out on one, two or three points and the calibration sequence can be chosen from a list of 13 buffers. The display shows continually the temperature in °C or °F and one of the parameters according to the connected probe type. Printing and storage always include the temperature in °C or °F and one selectable parameter for each probe type.

Other functions include: Max, Min and Avg function, the Auto-HOLD function, the automatic turning off which can also be excluded.

The instruments have IP66 protection degree.



Technical characteristics HD3405.2

pH - mV - °C/°F measurement

Instrument

Dimensions (Length x Width x Height)
Weight
Materials
Display

220x120x55mm
460g (complete with batteries)
ABS, rubber
2x4½ characters plus symbols
visible area: 52x42mm

Operating conditions

Working temperature
Storage temperature
Working relative humidity
Protection degree

-5 ... 50°C
-25 ... 65°C
0 ... 90% RH without condensation
IP66

Power

Batteries
Autonomy (only batteries)
Mains (cod. **SWD10**)

3 batteries 1.5V type AA
100 hours with 1800mAh alkaline batteries
Output mains adapter 100-240Vac/ 12Vdc-1A

Security of memorized data

Unlimited

Selectable storage interval

1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

Time

Date and hour
Accuracy

Schedule in real time
1min/month max departure

Serial interface RS232C

Type
Baud rate
Data bit
Parity
Stop bit
Flow Control
Serial cable length
Selectable print interval

RS232C electrically isolated
Can be set from 1200 to 38400 baud
8
None
1
Xon/Xoff
Max 15m
immediate or 1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

USB Interface

Type

1.1 - 2.0 electrically isolated

Connections

Serial interface and USB
Mains adapter (cod. **SWD10**)

8-pole MiniDin connector
2-pole connector (positive at centre) 12Vdc/1A

Storage of measured values


Type
Quantity

2000 pages of 17 samples each
34,000 sets of measures made up of [pH or mV] or and [°C or °F].

Measurement connections

Temperature probe input
with SICRAM module or TP47 module
pH/mV input

8-pole male DIN45326 connector
female BNC

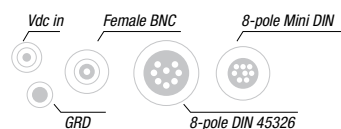

pH Measurement

Measurement range	-2.000...+19.999pH
Resolution	0.01 or 0.001pH selectable from menu
Accuracy	±0.001pH ±1digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	Offset! > 20mV Slope < 50mV/pH or Slope > 63mV/pH Sensitivity < 85% or Sensitivity > 106.5% -50...+150°C

Automatic / manual
temperature compensation

mV Measurement

Measurement range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	±0.1mV ±1digit
Drift after 1 year	0.5mV/year

Temperature Measurement

Pt100 measurement range	-200...+650°C
Pt1000 measurement range	-200...+650°C
Resolution	0.1°C
Accuracy	±0.1°C ±1digit
Drift after 1 year	0.1°C/year

Automatically detected pH standard solutions (@25°C)

1.679pH - 2.000pH - 4.000pH - 4.008pH
4.010pH - 6.860pH - 6.865pH - 7.000pH
7.413pH - 7.648pH - 9.180pH - 9.210pH
10.010pH

Ordering codes for instrument series HD34...

HD3405.2: The kit is composed of: instrument HD3405.2 **datalogger**, for measurement of pH - redox - temperature, 3 1.5V alkaline batteries, operating manual and **DeltaLog9 version 2.0**.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

Common Accessories for instruments series HD34...

HD2110CSNM: 8-pole connection cable Mini Din - Sub D 9-pole female for RS232C, for connection to PC without USB input.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole Mini Din for connection to PC with USB input.

SWD10: Stabilized power supply at 100-240Vac/12 Vdc-1A mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (**optional**) or supplier SWD10 (**optional**).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes to instrument series HD34..., without amplifying electronics and linearization.

pH Electrodes

KP20: Combined pH electrode for common use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for common use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. elektrolyte, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for common use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled with screw connector S7, body in glass.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

ORP Electrodes

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

Electrode dimensions and characteristics at page 402

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for refilling of the electrodes.

Cleaning and maintainance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Temperature probes complete with SICRAM module

TP87: Pt100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47module

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2 wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



pH



mV



HD 2205.2 BENCH-TOP pH METER

The **HD2205.2** is a bench top instruments for electrochemical measures: **pH** and **temperature**. It is fitted with a large backlit LCD display.

The **HD2205.2** is equipped with two BNC inputs for the measurement of **pH**, **mV**, **redox potential** (ORP) with pH or redox electrodes, or electrodes with separate reference, and one input for combined pH/temperature probes fitted with SICRAM module.

All models are fitted with input for the measurement of **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers.

- The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers. Temperature compensation can be automatic or manual.
- The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing parameters can be configured using the menu.
- The RS232C serial port can be used to transfer the acquired measurements to a 24 column portable printer in real time (HD40.1 or HD40.2).
- The instruments equipped with **HD22BT** (Bluetooth) option can transfer data without any connection to a PC or printer fitted with Bluetooth input or through Bluetooth/RS232C converter.
- The software DeltaLog11 allows instrument management and configuration, and data processing on PC.

The instruments have IP66 protection degree.

Technical characteristics HD2205.2

pH - mV - °C - °F measurement

Instrument

Dimensions (Length x Width x Height)	265x185x70mm
Weight	490g
Materials	ABS, rubber
Display	Back lighted, matrix point display. 240x64 points, visible area: 128x35mm

Operating conditions

Working temperature	-5 ... 50°C
Storing temperature	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensate

Protection degree

IP66

Power

Mains adapter (cod. SWD10)

12Vdc/1A

Auxiliary socket

For supplying of electrode holder with built-in stirrer HD22.2

Security of memorized data

Unlimited

Time

Date and hour

Real time schedule with backup battery E 3.6V - 1/2AA

Accuracy

1min/month max drift


Measured values storing

Quantity

2000 screens

Storage interval

1s ... 999s

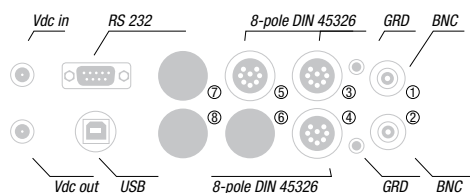

Calibration storage

Quantity	Last 8 calibrations of each physical quantity
----------	---

RS232C serial interface

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 115200 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Length of serial cable	Max 15m

USB Interface

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Bluetooth Interface

HD22BT optional

EMC standard regulations

Security	EN61000-4-2, EN61010-1 level 3
Electrostatic discharge	EN61000-4-2 level 3
Electric fast transients	EN61000-4-4 level 3, EN61000-4-5 level 3

Voltage variations

Electromagnetic interference susceptibility	IEC1000-4-3
---	-------------

Electromagnetic interference emission

EN55020 class B

Connections

Input for temperature probes with SICRAM module ③	8-pole male DIN45326 connector
Inputs pH/mV ① - ②	female BNC
Inputs for SICRAM module pH/temperature ③ a. ④	8-pole male DIN45326 connector
Serial interface	DB9 connector (9- pole male)
USB interface	USB connector type B
Bluetooth	Optional
Mains adapter	2- pole connector (Ø5.5mm-2.1mm). Positive at centre.
Socket for power supply of electrode holder with built-in magnetic stirrer	2 -pole connector (Ø5.5mm-2.1mm). Positive at centre (output 12Vdc/200mA max).

Measurement of pH by instrument

Measuring range	-9.999...+19.999pH
Resolution	0.01 o 0.001pH selectable from menu
Accuracy	±0.001pH ±1digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	IOffset1 > 20mV Slope > 63mV/pH o Slope < 50mV/pH Sensitivity > 106.5% or Sensitivity < 85%
Calibration points	Up to 5 points from a list of 13 automatically detected buffers.
Automatically detected pH standard solutions (@25°C)	1.679pH - 2.000pH - 4.000pH - 4.008pH - 4.010pH 6.860pH - 6.865pH - 7.000pH - 7.413pH - 7.648pH 9.180pH - 9.210pH - 10.010pH

Measurement of mV by instrument

Measuring range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	±0.1mV ±1digit
Drift after 1 year	0.5mV/year

Measurement of temperature by instrument

Pt100 Measuring range	-50...+150°C
Pt1000 Measuring range	-50...+150°C
Resolution	0.1°C
Accuracy	±0.1°C ±1digit
Drift after 1 year	0.1°C/year

ORDERING CODES

HD2205.2: The kit is composed of: instrument HD2205.2 for measurement of pH - redox - temperature, **data logger**, stabilized power supply at mains voltage 100-240Vac/12Vdc-1A., instructions manual and software DeltaLog11.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

ACCESSORIES

9CPRS232: Connection cable SubD female 9- pole for serial output RS232C.

CP22: USB 2.0 connection cable - connector type A - connector type B.

DeltaLog11: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.

HD40.1: 24-column portable thermal printer, serial interface, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

HD40.2: 24-column portable thermal printer, **Bluetooth and serial interface**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (**optional**) or the cable HD 2110 CSNM (**optional**).

HD2110CSP: Connection cable for instruments series HD34...to printer **S'print-BT**

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (**optional**) or supplier SWD10 (**optional**).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

HD22BT: Bluetooth module for wireless data transmission from instrument to PC. **The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.**

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD40.1



pH



mV

pH electrodes without SICRAM module (Inputs ① and ②)

KP20: Combined pH electrode for general use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for general use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. Liquid reference filling, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for general use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled, with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled, with screw connector S7, body in glass.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

pH electrodes with SICRAM module (Input③)

KP63TS: Combined pH/temperature electrode with SICRAM module, body in Epoxy, Ag/AgCl sat KCl.

SICRAM Module with BNC input for pH electrodes (Input ③)

KP47: SICRAM module for pH electrode with BNC standard connector.

ORP Electrodes (Inputs ① and ②)

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

Characteristics and dimensions of the probes at page 402

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for electrode refilling.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (tiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Temperature probes complete with SICRAM module (Input ⑤)

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47 module (input⑤)

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD22.2



HD 3456.2 BENCH-TOP pH AND CONDUCTIVITY METER

The HD3456.2 is a bench top instrument for electrochemical measures: **pH, conductivity and temperature**.

The displayed data can be stored (**datalogger**) and can be transferred to PC or serial printer thanks to the multi-standard serial port RS232C and USB2.0 and software DeltaLog9 (Vers.2.0 and subsequent ones). The storing and printing parameters can be set from menu.

The **HD3456.2** measures **pH, mV, redox potential (ORP), conductivity, resistivity in liquids, total dissolved solids (TDS), and salinity** using combined 4-ring and 2-ring conductivity/temperature probes. **Temperature** is measured by Pt100 or Pt1000 immersion, penetration or contact probes.

The pH electrode calibration, as well as manual, can be carried out automatically on one, two or three points and the calibration sequence can be chosen from a list of 13 buffers.

The conductivity probe calibration can be performed automatically in one or more of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions.



The display shows continually the temperature in °C or °F and one selectable parameter according to the connected probe type, i.e. in case of conductivity probe it is possible to select between χ or Ω or TDS or g/l.

Other functions of this instrument include: Max, Min and Avg function, the Auto-HOLD function, the automatic turning off which can also be disabled.

The instruments have IP66 protection degree.

Technical characteristics HD3456.2

pH, mV, χ , Ω , TDS, Sal, °C/°F measurement

Instrument

Dimensions (Length x Width x Height)	220x120x55mm
Weight	460g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ characters plus symbols visible area: 52x42mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% RH without condensation

Protection degree

IP66

Power

Batteries	3 batteries 1.5V type AA
Autonomy (only batteries)	100 hours with 1800mAh alkaline batteries
Mains (cod. SWD10)	Output mains adapter 100-240Vac/ 12Vdc-1A

Security of memorized data

Unlimited

Selectable storage interval

1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

Time

Date and hour	Schedule in real time
Accuracy	1min/month max drift

Serial interface RS232C


Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Selectable print interval	immediate or 1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1ora

USB Interface

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Connections

Serial interface and USB	8-pole MiniDin connector
Mains adapter (cod. SWD10)	2-pole connector (positive at centre) 12Vdc/1A

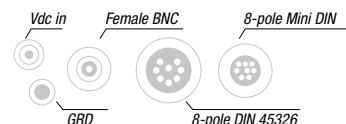

Storage of measured values

Tipo	2000 pages of 10 samples each
Quantity	20,000 terns of measures made up of [pH or mV], [X or Ω or TDS or salinity] and temperature.

Connections

pH/mV input	Female BNC connector
Conductivity input	8-pole male DIN45326 connector
Input for temperature probes with TP47 module	8-pole male DIN45326 connector

Measurement of pH by Instrument

Measurement range	-2.000...+19.999pH
Resolution	0.01 o 0.001pH selectable from menu
Accuracy	$\pm 0.001\text{pH} \pm 1\text{digit}$
Input impedance	$>10^{12}\Omega$
Calibration error @25°C	Offset $> 20\text{mV}$ Slope $> 63\text{mV/pH}$ or Slope $< 50\text{mV/pH}$ Sensitivity $> 106.5\%$ or Sensitivity $< 85\%$
Automatic / manual temperature compensation	-50...+150°C

Measurement of mV by Instrument

Measurement range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	$\pm 0.1\text{mV} \pm 1\text{digit}$
Drift after 1 year	0.5mV/year

Standard solutions automatically detected (@25°C)

1.679pH - 2.000pH - 4.000pH - 4.008pH
4.010pH - 6.860pH - 6.865pH - 7.000pH
7.413pH - 7.648pH - 9.180pH - 9.210pH
10.010pH

Measurement of conductivity by Instrument

		Resolution
Measurement range (Kcell=0.01)	0.000...1.999 $\mu\text{S/cm}$	0.001 $\mu\text{S/cm}$
Measurement range (Kcell=0.1)	0.00...19.99 $\mu\text{S/cm}$	0.01 $\mu\text{S/cm}$
Measurement range (Kcell=1)	0.0...199.9 $\mu\text{S/cm}$	0.1 $\mu\text{S/cm}$
	200...1999 $\mu\text{S/cm}$	1 $\mu\text{S/cm}$
	2.00...19.99mS/cm	0.01mS/cm
	20.0...199.9mS/cm	0.1mS/cm
Measurement range (Kcell=10)	200...1999mS/cm	1mS/cm
Accuracy (conductivity)	$\pm 0.5\% \pm 1\text{digit}$	

Measurement of resistivity by Instrument

		Resolution
Measurement range (Kcell=0.01)	Up to 1G $\Omega\text{-cm}$	(*)
Measurement range (Kcell=0.1)	Up to 100M $\Omega\text{-cm}$	(*)
Measurement range (Kcell=1)	5.0...199.9 $\Omega\text{-cm}$	0.1 $\Omega\text{-cm}$
	200...999 $\Omega\text{-cm}$	1 $\Omega\text{-cm}$

		Resolution
	1.00k...19.99k $\Omega\text{-cm}$	0.01k $\Omega\text{-cm}$
	20.0k...99.9k $\Omega\text{-cm}$	0.1k $\Omega\text{-cm}$
	100k...999k $\Omega\text{-cm}$	1k $\Omega\text{-cm}$
	1...10M $\Omega\text{-cm}$	1M $\Omega\text{-cm}$
Measurement range (Kcell=10) / Res.	0.5...5.0 $\Omega\text{-cm}$	0.1 $\Omega\text{-cm}$
Accuracy (resistivity)	$\pm 0.5\% \pm 1\text{digit}$	

Measurement of total dissolved solids (with coefficient X/TDS=0.5)

Measurement range (Kcell=0.01) / Res.	0.00...1.999mg/l	0.005mg/l
Measurement range (Kcell=0.1) / Res.	0.00...19.99mg/l	0.05mg/l
Measurement range (Kcell=1) / Res.	0.0...199.9 mg/l	0.5 mg/l
	200...1999 mg/l	1 mg/l
	2.00...19.99 g/l	0.01 g/l
	20.0...99.9 g/l	0.1 g/l
Measurement range (Kcell=10) / Res.	100...999 g/l	1 g/l
Accuracy (total dissolved solids)	$\pm 0.5\% \pm 1\text{digit}$	

Measurement of salinity

Measurement range / Resolution	0.000...1.999g/l	1 mg/l
	2.00...19.99g/l	10mg/l
	20.0...199.9g/l	0.1g/l
Accuracy (salinity)	$\pm 0.5\% \pm 1\text{digit}$	

Automatic/manual temperature compensation

0...100°C with α_t that can be selected from 0.00 to 4.00%/°C

Reference temperature

20°C o 25°C selectable from menu

X/TDS conversion factor

0.4...0.8

Cell constant K (cm⁻¹)

0.01 - 0.1 - 0.7 - 1.0 - 10.0

Standard solutions automatically detected (@25°C)

147 $\mu\text{S/cm}$
1413 $\mu\text{S/cm}$
12880 $\mu\text{S/cm}$
111800 $\mu\text{S/cm}$

Measurement of temperature by Instrument

Pt100 measurement range	-50...+200°C
Pt1000 measurement range	-50...+200°C
Resolution	0.1°C
Accuracy	$\pm 0.25^\circ\text{C}$
Drift after 1 year	0.1°C/year

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity ($\mu\text{S/cm}$)	Resistivity (M $\Omega\text{-cm}$)	Conductivity ($\mu\text{S/cm}$)	Resistivity(M $\Omega\text{-cm}$)
0.001 $\mu\text{S/cm}$	1000 M $\Omega\text{-cm}$	0.01 $\mu\text{S/cm}$	100 M $\Omega\text{-cm}$
0.002 $\mu\text{S/cm}$	500 M $\Omega\text{-cm}$	0.02 $\mu\text{S/cm}$	50 M $\Omega\text{-cm}$
0.003 $\mu\text{S/cm}$	333 M $\Omega\text{-cm}$	0.03 $\mu\text{S/cm}$	33 M $\Omega\text{-cm}$
0.004 $\mu\text{S/cm}$	250 M $\Omega\text{-cm}$	0.04 $\mu\text{S/cm}$	25 M $\Omega\text{-cm}$
...



pH



X



Ω



TDS

ORDERING CODES

HD3456.2: The kit is composed of: instrument HD3456.2 **datalogger**, for the measurement of pH - redox - conductivity - resistivity - TDS - salinity - temperature, 3 1.5V alkaline batteries, operating manual and **DeltaLog9 version 2.0**.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

ACCESSORIES

HD2110CSNM: 8-pole connection cable Mini Din - Sub D 9-pole female for RS232C, for connection to PC without USB input.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole Mini Din for connection to PC with USB input.

SWD10: Stabilized power supply at 230Vac/9Vdc-300mA mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD2110CSP: Connection cable for instruments series HD34... to printer **S'print-BT**

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

pH Electrodes

KP20: Combined pH electrode for common use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for common use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. electrolyte, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for common use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled with screw connector S7, body in glass.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

ORP Electrodes

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for refilling of the electrodes.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Combined conductivity and temperature probes

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant $K = 0.7$. Measurement range $5\mu\text{S}/\text{cm} \dots 200\text{mS}/\text{cm}$, $0 \dots 90^\circ\text{C}$.

SPT401.001: Combined conductivity and temperature 2-electrode cell in stainless steel AISI 316. Cell constant $K = 0.01$. Measurement range $0.04\mu\text{S}/\text{cm} \dots 20\mu\text{S}/\text{cm}$, $0 \dots 120^\circ\text{C}$. Measurement in closed-cell..

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant $K = 0.1$. Measurement range $0.1\mu\text{S}/\text{cm} \dots 500\mu\text{S}/\text{cm}$, $0 \dots 80^\circ\text{C}$.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant $K = 1$. Measurement range $10\mu\text{S}/\text{cm} \dots 10\text{mS}/\text{cm}$, $0 \dots 80^\circ\text{C}$.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant $K = 10$. Measurement range $500\mu\text{S}/\text{cm} \dots 200\text{mS}/\text{cm}$, $0 \dots 80^\circ\text{C}$.

Electrode dimensions and characteristics at page 402

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to $147\mu\text{S}/\text{cm}$ @ 25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to $1413\mu\text{S}/\text{cm}$ @ 25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to $12880\mu\text{S}/\text{cm}$ @ 25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to $111800\mu\text{S}/\text{cm}$ @ 25°C - 200cc.

Temperature probes complete with TP47 module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2 wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.





HD 2256.2 BENCH-TOP pH AND CONDUCTIVITY METER

The **HD2256.2** is a bench top instrument for electrochemical measures: **pH**, **conductivity** and **temperature**. It is fitted with a large backlit LCD display. The **HD2256.2** measures **pH**, **mV**, **redox potential** (ORP) with pH, redox electrodes or electrodes with separate reference. **Conductivity and resistivity** in liquids, **total dissolved solids** (TDS) and **salinity** with combined 4-ring and 2-ring conductivity/temperature probes. The conductivity probes can have a direct input or with SICRAM module. The inputs are separate. All models are fitted with input for the measurement of **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

- The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers Temperature compensation can be automatic or manual.
- The conductivity probe calibration can be performed automatically with automatically detected conductivity calibration solutions: 147µS/cm, 1413µS/cm, 12880µS/cm or 111800µS/cm or manually with calibration solutions having different values.
- Conductivity, dissolved oxygen and temperature probes fitted with SICRAM module can store factory and calibration data inside.

The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing parameters can be configured using the menu. The RS232C serial port can be used to transfer the acquired measurements to a 24 column portable printer in real time (HD40.1 or HD40.2).

The instruments equipped with **HD22BT** (Bluetooth) option can transfer data without any connection to a PC or printer fitted with Bluetooth input or through Bluetooth/RS232C converter. The software DeltaLog11 allows instrument management and configuration, and data processing on PC.

The instruments have IP66 protection degree.

Technical characteristics HD2256.2

pH - mV - χ - Ω - TDS - NaCl - °C - °F

Instrument

Dimensions (Length x Width x Height)	265x185x70mm
Weight	490g
Materials	ABS, rubber
Display	Back lighted, matrix point display. 240x64 points, visible area: 128x35mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensate
Protection degree	IP66

Power

	Mains adapter (cod. SWD10) 12Vdc/1A
Auxiliary socket	For supplying of electrode holder with built-in stirrer HD22.2

Security of memorized data


Unlimited

Time

Date and hour	Real time schedule with backup battery 3.6V - ½AA
Accuracy	1min/month max drift

Measured values storing

Quantity	2000 screens
Storage interval	1s ... 999s

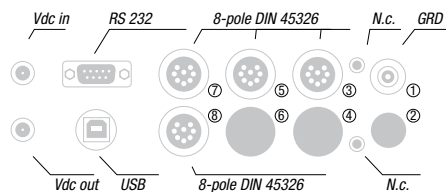

<i>Calibration storage</i>	
Quantity	Last 8 calibrations of each physical quantity

RS232C serial interface

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 115200 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Length of serial cable	Max 15m

USB Interface

Type	1.1 - 2.0 electrically isolated
Bluetooth Interface	optional

Connections

Input for temperature probes with SICRAM modules⑤	8-pole male DIN45326 connector
pH/mV input ①	BNC female
Input for SICRAM module pH/ temperature ③	8-pole male DIN45326 connector
2/ 4- electrode direct conductivity input ⑧	8-pole male DIN45326 connector
Input conductivity electrodes with SICRAM module⑦	8-pole male DIN45326 connector
Serial interface	DB9 connector (9- pole male)
USB interface	USB connector type B
Bluetooth	Optional
Mains adapter	2-pole connector (Ø5.5mm-2.1mm). Positive at centre
Outlet for power supply of electrode holder with built-in magnetic stirrer	2-pole connector (Ø5.5mm-2.1mm). Positive at centre (output 12Vdc/200mA max).

pH measurement by instrument

Measuring range	-9.999...+19.999pH
Resolution	0.01 o 0.001pH selectable from menu
Accuracy	±0.001pH ±1digit
Input impedance	>10 ¹² Ω
Calibration error @25°C	Offset1 > 20mV Slope > 63mV/pH o Slope < 50mV/pH Sensitivity > 106.5% or Sensitivity < 85%
Calibration points	Up to 5 points with 13 automatically detected buffer solutions
Standard solutions automatically detected (@25°C)	1.679pH - 2.000pH - 4.000pH - 4.008pH 4.010pH - 6.860pH - 6.865pH - 7.000pH 7.413pH - 7.648pH - 9.180pH - 9.210pH 10.010pH

mV measurement by instrument

Measuring range	-1999.9...+1999.9mV
Resolution	0.1mV
Accuracy	±0.1mV ±1digit
Drift after 1 year	0.5mV/year

Conductivity measurement by instrument

Measuring range (Kcell=0.01) / Res.	0.000...1.999μS/cm	Resolution	0.001μS/cm
Measuring range (Kcell=0.1) / Res.	0.00...19.99μS/cm		0.01μS/cm
Measuring range (K cell=1) / Res.	0.0...199.9μS/cm		0.1μS/cm
	200...1999μS/cm		1μS/cm
	2.00...19.99mS/cm		0.01mS/cm
	20.0...199.9mS/cm		0.1mS/cm
Measuring range (Kcell=10) / Res.	200...1999mS/cm		1mS/cm
Accuracy (conductivity)	±0.5% ±1digit		

Measurement of resistivity by instrument

Measuring range (Kcell=0.01)	Up to 1GΩ·cm	Resolution	(*)
Measuring range (Kcell=0.1)	Up to 100MΩ·cm		(*)
Measuring range (K cell=1)	5.0...199.9Ω·cm		0.1Ω·cm
	200...999Ω·cm		1Ω·cm
	1.00k...19.99kΩ·cm		0.01kΩ·cm
	20.0k...99.9kΩ·cm		0.1kΩ·cm
	100k...999kΩ·cm		1kΩ·cm
	1...10MΩ·cm		1MΩ·cm
Measuring range (Kcell=10)	0.5...5.0Ω·cm		0.1Ω·cm
Accuracy (resistivity)	±0.5% ±1digit		

Measurement of total dissolved solids (with coefficient χ /TDS=0.5)

Measuring range (Kcell=0.01)	0.00...1.999mg/l	0.005mg/l
Measuring range (Kcell=0.1)	0.00...19.99mg/l	0.05mg/l
Measuring range (K cell=1)	0.0...199.9 mg/l	0.5 mg/l
	200...1999 mg/l	1 mg/l
	2.00...19.99 g/l	0.01 g/l
	20.0...199.9 g/l	0.1 g/l
Measuring range (Kcell=10)	100...999 g/l	1 g/l
Accuracy (total dissolved solids)	±0.5% ±1digit	

Measurement of salinity by instrument

Measuring range	0.000...1.999g/l	1mg/l
	2.00...19.99g/l	10mg/l
	20.0...199.9 g/l	0.1 g/l
Accuracy (salinity)	±0.5% ±1digit	

Automatic/manual temperature compensation

	0...100°C with $\alpha_T = 0.00...4.00\%/^{\circ}\text{C}$
Reference temperature	0...50°C
Conversion factor χ /TDS	0.4...0.8
Cell constant K (cm ⁻¹) already set on instrument	0.01 - 0.1 - 0.5 - 0.7 - 1.0 - 10.0
Cell constants K(cm ⁻¹) that can be set by user	0.01...20.00

Standard solutions automatically detected (@25°C)

	147μS/cm
	1413μS/cm
	12880μS/cm
	111800μS/cm

Measurement of temperature by instrument

Pt100 measuring range	-50...+150°C
Pt1000 measuring range	-50...+150°C
Resolution	0.1°C
Accuracy ±0.1°C ±1digit	
Drift after 1 year	0.1°C/year

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity (μS/cm)	Resistivity (MΩ·cm)	Conductivity (μS/cm)	Resistivity(MΩ·cm)
0.001 μS/cm	1000 MΩ·cm	0.01 μS/cm	100 MΩ·cm
0.002 μS/cm	500 MΩ·cm	0.02 μS/cm	50 MΩ·cm
0.003 μS/cm	333 MΩ·cm	0.03 μS/cm	33 MΩ·cm
0.004 μS/cm	250 MΩ·cm	0.04 μS/cm	25 MΩ·cm
...

ORDERING CODES

HD2256.2: The kit is composed of: instrument HD2256.2 for the measurement of pH - redox - conductivity - resistivity - TDS - salinity - temperature, **datalogger**, stabilized power supply at mains voltage 100-240Vac/12Vdc-1A., instructions manual and software Del-taLog11.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

ACCESSORIES

9CPRS232: Connection cable SubD female 9- pole for serial output RS232C.

CP22: USB 2.0 connection cable - connector type A - connector type B.

DeltaLog11: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply at 230Vac/9Vdc-300mA mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD40.2: 24-column portable thermal printer, **Bluetooth and serial interface**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (optional) or the cable HD 2110 CSNM (optional).

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

HD22BT: Bluetooth module for wireless data transmission from instrument to PC. **The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.**

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

pH electrodes without SICRAM module (Inputs ① and ②)

KP20: Combined pH electrode for general use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for general use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. Liquid reference filling, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for general use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled, with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled, with screw connector S7, body in glass.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

pH electrodes with SICRAM module (Input ③)

KP63TS: Combined pH/temperature electrode with SICRAM module, body in Epoxy, Ag/AgCl sat KCl.

SICRAM Module with BNC input for pH electrodes (Input ③)

KP47: SICRAM module for pH electrode with BNC standard connector.

Electrode characteristics at page 401

ORP Electrodes (Inputs ① and ②)

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for electrode refilling.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (tiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Conductivity probes and combined conductivity and temperature probes without SICRAM module (Input ⑦)

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant K = 0.7. Measurement range 5µS/cm ...200mS/cm, 0...90°C.

SPT401.001: Combined conductivity and temperature 2- electrode cell in stainless steel AISI 316. Cell constant K = 0.01. Measurement range 0.04µS/cm ...20µS/cm, 0...120°C. Measurement in closed-cell.

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 0.1. Measurement range 0.1µS/cm ...500µS/cm, 0...80°C.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 1. Measurement range 10µS/cm ...10mS/cm, 0...80°C.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 10. Measurement range 500µS/cm ...200mS/cm, 0...80°C.

Combined conductivity / temperature probes with SICRAM module (Input ⑧)

SPT1GS: Combined conductivity /temperature 2-electrode Platinum- wire cell, body in glass with SICRAM module. Cell constant K = 1. Measuring range 10µS/cm ...10mS/cm, 0...80°C.

Electrode characteristics at page 402

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147µS/cm @25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413µS/cm @25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880µS/cm @25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800µS/cm @25°C - 200cc.

Temperature probes compete with SICRAM module (Input ⑤)

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47 module (input ⑤)

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



X



mV

Instrument

Dimensions (Length x Width x Height)
Weight
Materials
Display

220x120x55mm
460g (complete with batteries)
ABS, rubber
2x4½ characters plus symbols
visible area: 52x42mm

Operating conditions

Working temperature
Storage temperature
Working relative humidity

-5 ... 50°C
-25 ... 65°C
0 ... 90% RH without condensation

Protection degree

IP66

Power

Batteries
Autonomy (only batteries)
Mains (cod. **SWD10**)

3 batteries 1.5V type AA
100 hours with 1800mAh alkaline batteries
Output mains adapter 100-240Vac/ 12Vdc-1A

Security of memorized data

Unlimited

Selectable storage interval

1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

Time

Date and hour
Accuracy

Schedule in real time
1min/month max drift

Serial interface RS232C

Type
Baud rate
Data bit
Parity
Stop bit
Flow Control
Serial cable length
Selectable print interval

RS232C electrically isolated
Can be set from 1200 to 38400 baud
8
None
1
Xon/Xoff
Max 15m
immediate or 1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

USB Interface

Type

1.1 - 2.0 electrically isolated

Common connections to all models

Serial interface and USB
Mains adapter (cod. **SWD10**)

8-pole MiniDin connector
2-pole connector (positive at centre) 12Vdc/1A

Storage of measured values

Type
Quantity

2000 pages of 18 samples each
36,000 sets of measures made up of [χ - Ω or TDS or NaCl] and [°C - °F]

Measurement connections

Input conductivity
Input for temperature probes
complete with TP47 modules

8-pole male DIN45326 connector
8-pole male DIN45326 connector

Measurement of conductivity by instrument

Measurement range (Kcell=0.01)
Measurement range (Kcell=0.1)
Measurement range (Kcell=1)

Measurement range	Resolution
0.000...1.999µS/cm	0.001µS/cm
0.00...19.99µS/cm	0.01µS/cm
0.0...199.9µS/cm	0.1µS/cm
200...1999µS/cm	1µS/cm
2.00...19.99mS/cm	0.01mS/cm
20.0...199.9mS/cm	0.1mS/cm



HD 3406.2 BENCH-TOP CONDUCTIVITY METER

The **HD3406.2** is a bench top instrument for electrochemical measures: **conductivity and temperature**.

The displayed data can be stored (**datalogger**) and can be transferred to PC or serial printer thanks to the multi-standard serial port RS232C and USB2.0 and software DeltaLog9 (Vers.2.0 and subsequent ones). The storing and printing parameters can be set from menu.


The **HD3406.2** measures **conductivity, liquid resistivity in liquids, total dissolved solids (TDS)** and **salinity** using combined 4-ring and 2-ring conductivity/temperature probes. Temperature is measured by Pt100 or Pt1000 immersion, penetration or contact probes.

The probe calibration can be performed automatically in one or more of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions.

The display shows continually the temperature in °C or °F and one selectable parameter according to the connected probe type, i.e. in case of conductivity probe it is possible to select between χ or Ω or TDS or NaCl.

Other functions of this instrument include: Max, Min and Avg function, the Auto-HOLD function, the automatic turning off which can also be excluded.

The instruments have IP66 protection degree.

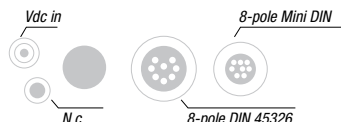

Range di misura (Kcell=10). 200...1999mS/cm 1mS/cm
Accuracy (conductivity) $\pm 0.5\% \pm 1$ digit

Measurement of resistivity by instrument

Measurement range (Kcell=0.01) Up to 1G Ω -cm (*)
Measurement range (Kcell=0.1) Up to 100M Ω -cm (*)
Measurement range (Kcell=1) 5.0...199.9 Ω -cm 0.1 Ω -cm
200...999 Ω -cm 1 Ω -cm
1.00k...19.99k Ω -cm 0.01k Ω -cm
20.0k...99.9k Ω -cm 0.1k Ω -cm
100k...999k Ω -cm 1k Ω -cm
1...10M Ω -cm 1M Ω -cm
Measurement range (Kcell=10) 0.5...5.0 Ω -cm 0.1 Ω -cm
Accuracy (resistivity) $\pm 0.5\% \pm 1$ digit

Measurement of total dissolved solids (with coefficient χ /TDS=0.5)

Measurement range (Kcell=0.01) 0.00...1.999mg/l 0.005mg/l
Measurement range (Kcell=0.1) 0.00...19.99mg/l 0.05mg/l
Measurement range (Kcell=1) 0.0...199.9 mg/l 0.5 mg/l
200...1999 mg/l 1 mg/l
2.00...19.99 g/l 0.01 g/l
20.0...99.9 g/l 0.1 g/l
100...999 g/l 1 g/l
Measurement range (Kcell=10) 100...999 g/l 1 g/l
Accuracy (total dissolved solids) $\pm 0.5\% \pm 1$ digit

Measurement of salinity

Measurement range / Resolution 0.000...1.999g/l 1mg/l
2.00...19.99g/l 10mg/l
20.0...199.9g/l 0.1g/l
Accuracy (salinity) $\pm 0.5\% \pm 1$ digit

Temperature measurement by instrument

Measurement range Pt100 -50...+200°C
Measurement range Pt1000 -50...+200°C
Resolution 0.1°C
Accuracy $\pm 0.25^\circ\text{C}$
Drift after 1 year 0.1°C/year

Automatic/manual temperature compensation

Reference temperature 0...100°C with $\alpha_T = 0.00...4.00\%/^\circ\text{C}$
Conversion factor χ /TDS 20°C or 25°C selectable from menu
Cell constant K (cm⁻¹) 0.4...0.8
0.01 - 0.1 - 0.7 - 1.0 - 10.0

Standard solutions automatically detected (@25°C)

147 $\mu\text{S}/\text{cm}$
1413 $\mu\text{S}/\text{cm}$
12880 $\mu\text{S}/\text{cm}$
111800 $\mu\text{S}/\text{cm}$

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity ($\mu\text{S}/\text{cm}$)	Resistivity (M Ω -cm)	Conductivity ($\mu\text{S}/\text{cm}$)	Resistivity(M Ω -cm)
0.001 $\mu\text{S}/\text{cm}$	1000 M Ω -cm	0.01 $\mu\text{S}/\text{cm}$	100 M Ω -cm
0.002 $\mu\text{S}/\text{cm}$	500 M Ω -cm	0.02 $\mu\text{S}/\text{cm}$	50 M Ω -cm
0.003 $\mu\text{S}/\text{cm}$	333 M Ω -cm	0.03 $\mu\text{S}/\text{cm}$	33 M Ω -cm
0.004 $\mu\text{S}/\text{cm}$	250 M Ω -cm	0.04 $\mu\text{S}/\text{cm}$	25 M Ω -cm
...

ORDERING CODES

HD3406.2: The kit is composed of: instrument HD3406.2 **datalogger**, for measurement of conductivity - resistivity - TDS - salinity - temperature, 3 1.5V alkaline batteries, operating manual and **DeltaLog9 version 2.0**.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

ACCESSORIES

HD2110CSNM: 8-pole connection cable Mini Din - Sub D 9-pole female for RS232C, for connection to PC without USB input.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole Mini Din for connection to PC with USB input.

SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm.

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For \varnothing 12mm probes.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

Combined conductivity and temperature probes

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant K = 0.7. Measurement range 5 $\mu\text{S}/\text{cm}$...200mS/cm, 0...90°C.

SPT401.001: Combined conductivity and temperature 2- electrode cell in stainless steel AISI 316. Cell constant K = 0.01. Measurement range 0.04 $\mu\text{S}/\text{cm}$...20 $\mu\text{S}/\text{cm}$, 0...120°C. Measurement in closed-cell..

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 0.1. Measurement range 0.1 $\mu\text{S}/\text{cm}$...500 $\mu\text{S}/\text{cm}$, 0...80°C.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 1. Measurement range 10 $\mu\text{S}/\text{cm}$...10mS/cm, 0...80°C.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 10. Measurement range 500 $\mu\text{S}/\text{cm}$...200mS/cm, 0...80°C.

Electrode characteristics at page 402

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147 $\mu\text{S}/\text{cm}$ @25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413 $\mu\text{S}/\text{cm}$ @25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880 $\mu\text{S}/\text{cm}$ @25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800 $\mu\text{S}/\text{cm}$ @25°C - 200cc.

Temperature probes complete with TP47 module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem \varnothing 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem \varnothing 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem \varnothing 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem \varnothing 3mm, length 70mm. 2 wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



χ



Ω



mg/l



NaCl



HD 2206.2 BENCH-TOP CONDUCTIVITY METER

The **HD2206.2** is a bench top instrument for electrochemical measures: **conductivity**, and **temperature**. It is fitted with a large backlit LCD display.

The **HD2206.2** measures **conductivity**, **resistivity** in liquids, **total dissolved solids** (TDS), and **salinity** with combined 4-ring and 2-ring conductivity/temperature probes. The conductivity probes can have a direct input or with SICRAM module. The inputs are separate.

All models are fitted with input for the measurement of **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

- The conductivity probe calibration can be performed automatically with automatically detected conductivity calibration solutions: 147µS/cm, 1413µS/cm, 12880µS/cm or 111800µS/cm or manually with calibration solutions having different values.

- Conductivity, dissolved oxygen and temperature probes fitted with SICRAM module can store factory and calibration data inside.

The instruments HD2206.2 is a **datalogger**, it can memorize up to 2,000 samples of data. The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing parameters can be configured using the menu. The RS232C serial port can be used to transfer the acquired measurements to a 24 column portable printer in real time (HD40.1 or HD40.2).

The instruments equipped with **HD22BT** (Bluetooth) option can transfer data without any connection to a PC or printer fitted with Bluetooth input or through Bluetooth/RS232C converter. The software DeltaLog11 allows instrument management and configuration, and data processing on PC.

The instruments have IP66 protection degree.

Technical characteristics HD2206.2

X - Ω - TDS - NaCl - °C - °F measurement

Instrument

Dimensions (Length x Width x Height)	265x185x70mm
Weight	490g
Materials	ABS, rubber
Display	Back lighted, matrix point display. 240x64 points, visible area: 128x35mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensate

Protection degree

IP66

Power

Mains adapter (cod. SWD10)
12Vdc/1A

Auxiliary socket

For supplying of electrode holder with built-in stirrer HD22.2

Security of memorized data

Unlimited

Time

Date and hour


Real time schedule with backup battery 3.6V - ½AA

Accuracy

1min/month max drift

Measured values storing

Quantity	2000 screens
Storage interval	1s ... 999s

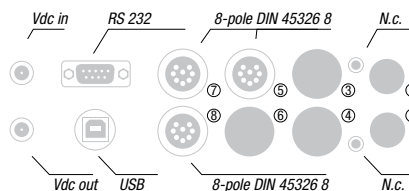

Calibration storage	
Quantity	Last 8 calibrations of each physical quantity
RS232C serial interface	
Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 115200 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Length of serial cable	Max 15m
USB Interface	
Type	1.1 - 2.0 electrically isolated
Bluetooth Interface	
	optional
Connections	
Input for temperature probes with SICRAM module ⑤	8-pole male DIN45326 connector
2/4 ring direct ③ conductivity input	8-pole male DIN45326 connector
Conductivity probe with SICRAM module input ⑦	8-pole male DIN45326 connector
Serial interface	DB9 connector (9- pole male)
USB interface	USB connector type B
Bluetooth	Optional
Mains adapter	2 -pole (Ø5.5mm-2.1mm). Positive at centre
Socket for power supply of electrode holder with built-in magnetic stirrer	2- pole connector (Ø5.5mm-2.1mm). Positive at centre (output 12Vdc/200mA max).

Measurement of conductivity by instrument		Resolution
Measuring range (Kcell=0.01)	0.000...1.999µS/cm	0.001µS/cm
Measuring range (Kcell=0.1)	0.00...19.99µS/cm	0.01µS/cm
Measuring range (K cell=1)	0.0...199.9µS/cm	0.1µS/cm
	200...1999µS/cm	1µS/cm
	2.00...19.99mS/cm	0.01mS/cm
	20.0...199.9mS/cm	0.1mS/cm
	200...1999mS/cm	1mS/cm
Measuring range (Kcell=10)	200...1999mS/cm	1mS/cm
Accuracy (conductivity)	±0.5% ±1digit	

<i>Measurement of resistivity by instrument</i>		
Measuring range (Kcell=0.01)	Up to 1GΩ·cm	(*)
Measuring range (Kcell=0.1)	Up to 100MΩ·cm	(*)
Measuring range (K cell=1)	5.0...199.9Ω·cm	0.1Ω·cm
	200...999Ω·cm	1Ω·cm
	1.00k...19.99kΩ·cm	0.01kΩ·cm
	20.0k...99.9kΩ·cm	0.1kΩ·cm
	100k...999kΩ·cm	1kΩ·cm
	1...10MΩ·cm	1MΩ·cm
	0.5...5.0Ω·cm	0.1Ω·cm
Measuring range (Kcell=10)	0.5...5.0Ω·cm	0.1Ω·cm
Accuracy (resistivity)	±0.5% ±1digit	

Measurement of total dissolved solids (with coefficient χ/TDS=0.5)		
Measuring range (Kcell=0.01)	0.00...1.999mg/l	0.005mg/l
Measuring range (Kcell=0.1)	0.00...19.99mg/l	0.05mg/l
Measuring range (K cell=1)	0.0...199.9 mg/l	0.5 mg/l
	200...1999 mg/l	1 mg/l
	2.00...19.99 g/l	0.01 g/l
	20.0...199.9 g/l	0.1 g/l
Measurement range (Kcell=10)	100...999 g/l	1 g/l
Accuracy (total dissolved solids)	±0.5% ±1digit	


Measurement of salinity		Resolution
Measuring range	0.000...1.999g/l	1mg/l
	2.00...19.99g/l	10mg/l
	20.0...199.9 g/l	0.1 g/l
Accuracy (salinity)	±0.5% ±1digit	
Automatic/manual temperature compensation		0...100°C with $\alpha_T = 0.00...4.00\%/^{\circ}\text{C}$
Reference temperature	0...50°C	
χ /TDS conversion factor	0.4...0.8	
Cell constants K (cm ⁻¹) already set on the instrument	0.01 - 0.1 - 0.5 - 0.7 - 1.0 - 10.0	
Cell constants K(cm ⁻¹) that can be set by user	0.01...20.00	

Standard solutions automatically detected (@25°C)	
	147µS/cm
	1413µS/cm
	12880µS/cm
	111800µS/cm

Measurement of temperature by instrument	
Pt100 measuring range	-50...+150°C
Pt1000 measuring range	-50...+150°C
Resolution	0.1°C
Accuracy	±0.1°C ±1digit
Drift after 1 year	0.1°C/year

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity (µS/cm)	Resistivity (MΩ·cm)	Conductivity (µS/cm)	Resistivity (MΩ·cm)
0.001 µS/cm	1000 MΩ·cm	0.01 µS/cm	100 MΩ·cm
0.002 µS/cm	500 MΩ·cm	0.02 µS/cm	50 MΩ·cm
0.003 µS/cm	333 MΩ·cm	0.03 µS/cm	33 MΩ·cm
0.004 µS/cm	250 MΩ·cm	0.04 µS/cm	25 MΩ·cm
...

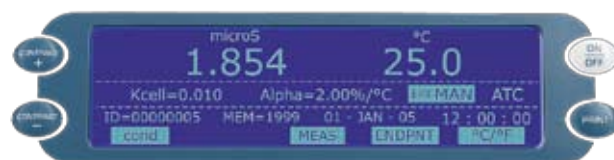

χ



TDS

ORDERING CODES

HD2206.2: The kit is composed of: instrument HD2206.2 for the measurement of conductivity - resistivity - TDS - salinity - temperature, **data logger**, stabilized power supply at mains voltage 100-240Vac/12Vdc-1A., instructions manual and software DeltaLog11.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

ACCESSORIES

9CPRS232: Connection cable SubD female 9- pole for serial output RS232C.

CP22: USB 2.0 connection cable - connector type A - connector type B.

DeltaLog11: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply at 230Vac/12Vdc-1A mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD40.2: 24-column portable thermal printer, **Bluetooth and serial interface**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (optional) or the cable HD 2110 CSNM (optional).

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

HD22BT: Bluetooth module for wireless data transmission from instrument to PC. **The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.**

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

Conductivity probes and combined conductivity and temperature probes without SICRAM module (Input Ⓢ)

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant K = 0.7. Measurement range 5µS/cm ...200mS/cm, 0...90°C.

SPT401.001: Combined conductivity and temperature 2- electrode cell in stainless steel AISI 316. Cell constant K = 0.01. Measurement range 0.04µS/cm ...20µS/cm, 0...120°C. Measurement in closed-cell.

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 0.1. Measurement range 0.1µS/cm ...500µS/cm, 0...80°C.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 1. Measurement range 10µS/cm ...10mS/cm, 0...80°C.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 10. Measurement range 500µS/cm ...200mS/cm, 0...80°C.

Electrode dimensions and characteristics at page 402

Combined conductivity / temperature probes with SICRAM module (Input Ⓢ)

SPT1GS: Combined conductivity /temperature 2-electrode Platinum- wire cell, body in glass with SICRAM module. Cell constant K = 1. Measuring range 10µS/cm ...10mS/cm, 0...80°C.

Electrode dimensions and characteristics at page 402

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147µS/cm @25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413µS/cm @25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880µS/cm @25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800µS/cm @25°C - 200cc.

Temperature probes complete with SICRAM module (Input Ⓢ)

TP87: Pt100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47 module (input Ⓢ)

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD40.1



HD22.3



HD 3456.2 BENCH-TOP CONDUCTIVITY AND pH METER

The **HD3456.2** is a bench top instrument for electrochemical measures: **pH, conductivity and temperature.**

The displayed data can be stored (**datalogger**) and can be transferred to PC or serial printer thanks to the multi-standard serial ports RS232C and USB2.0 and software DeltaLog9

The **HD3456.2** measures **pH, mV, redox potential (ORP), conductivity, resistivity in liquids, total dissolved solids (TDS), and salinity** using combined 4-ring and 2-ring conductivity/temperature probes. **Temperature** is measured by Pt100 or Pt1000 immersion, penetration or contact probes.

The pH electrode calibration, as well as manual, can be carried out on one, two or three points and the calibration sequence can be chosen from a list of 13 buffers.

The probe calibration can be performed automatically in one or more of the 147µS, 1413µS, 12880µS or 111800µS/cm conductivity calibration solutions.

The display shows continually the temperature in °C or °F and one selectable parameter according to the connected probe type, i.e. in case of conductivity probe it is possible to select between χ or Ω or TDS or NaCl.



Other functions of this instrument include: Max, Min and Avg function, the Auto-HOLD function, the automatic turning off which can also be excluded.

The instruments have IP66 protection degree.

Technical characteristics HD3456.2

pH, mV, χ , Ω , TDS, Sal, °C/°F measurement

Instrument

Dimensions (Length x Width x Height)	220x120x55mm
Weight	460g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ characters plus symbols visible area: 52x42mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% RH without condensation
Protection degree	IP66

Power

Batteries	3 batteries 1.5V type AA
Autonomy (only batteries)	100 hours with 1800mAh alkaline batteries
Mains (cod. SWD10)	Output mains adapter 100-240Vac/ 12Vdc-1A

Security of memorized data

Unlimited

Selectable storage interval

1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

Time


Date and hour	Schedule in real time
Accuracy	1min/month max drift

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Selectable print interval	immediate or 1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

USB Interface

Type	1.1 - 2.0 electrically isolated
------	---------------------------------

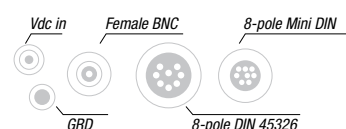

Connections
 Serial interface and USB 8-pole MiniDin connector
 Mains adapter (cod. SWD10) 2-pole connector (positive at centre) 12Vdc/1A

Storage of measured values
 Tipo 2000 pages of 10 samples each
 Quantity 20,000 turns of measures made up of [pH or mV], [X or Ω or TDS or salinity] and temperature.

Connections
 pH/mV input Female BNC connector
 Conductivity input 8-pole male DIN45326 connector
 Input for temperature probes with TP47 module 8-pole male DIN45326 connector

Measurement of pH by Instrument
 Measurement range -2.000...+19.999pH
 Resolution 0.01 o 0.001pH selectable from menu
 Accuracy $\pm 0.001\text{pH} \pm 1\text{digit}$
 Input impedance $>10^{12}\Omega$
 Calibration error @25°C Offset $> 20\text{mV}$
 Slope $> 63\text{mV/pH}$ or Slope $< 50\text{mV/pH}$
 Sensitivity $> 106.5\%$ or Sensitivity $< 85\%$
 Automatic / manual -50...+150°C
 temperature compensation

Measurement of mV by Instrument
 Measurement range -1999.9...+1999.9mV
 Resolution 0.1mV
 Accuracy $\pm 0.1\text{mV} \pm 1\text{digit}$
 Drift after 1 year 0.5mV/year

Standard solutions automatically detected (@25°C)
 1.679pH - 2.000pH - 4.000pH - 4.008pH - 4.010pH
 6.860pH - 6.865pH - 7.000pH - 7.413pH - 7.648pH
 9.180pH - 9.210pH - 10.010pH

Measurement of conductivity by Instrument
 Measurement range (Kcell=0.01) 0.000...1.999 $\mu\text{S/cm}$ 0.001 $\mu\text{S/cm}$
 Measurement range (Kcell=0.1) 0.00...19.99 $\mu\text{S/cm}$ 0.01 $\mu\text{S/cm}$
 Measurement range (Kcell=1) 0.0...199.9 $\mu\text{S/cm}$ 0.1 $\mu\text{S/cm}$
 200...1999 $\mu\text{S/cm}$ 1 $\mu\text{S/cm}$
 2.00...19.99mS/cm 0.01mS/cm
 20.0...199.9mS/cm 0.1mS/cm
 Measurement range (Kcell=10) 200...1999mS/cm 1mS/cm
 Accuracy (conductivity) $\pm 0.5\% \pm 1\text{digit}$

Measurement of resistivity by Instrument
 Measurement range (Kcell=0.01) Up to 1G $\Omega\cdot\text{cm}$ (*)
 Measurement range (Kcell=0.1) Up to 100M $\Omega\cdot\text{cm}$ (*)
 Measurement range (Kcell=1) 5.0...199.9 $\Omega\cdot\text{cm}$ 0.1 $\Omega\cdot\text{cm}$
 200...999 $\Omega\cdot\text{cm}$ 1 $\Omega\cdot\text{cm}$
 1.00k...19.99k $\Omega\cdot\text{cm}$ 0.01k $\Omega\cdot\text{cm}$
 20.0k...99.9k $\Omega\cdot\text{cm}$ 0.1k $\Omega\cdot\text{cm}$
 100k...999k $\Omega\cdot\text{cm}$ 1k $\Omega\cdot\text{cm}$
 1...10M $\Omega\cdot\text{cm}$ 1M $\Omega\cdot\text{cm}$
 Measurement range (Kcell=10) 0.5...5.0 $\Omega\cdot\text{cm}$ 0.1 $\Omega\cdot\text{cm}$
 Accuracy (resistivity) $\pm 0.5\% \pm 1\text{digit}$

Measurement of total dissolved solids (with coefficient $\chi/\text{TDS}=0.5$)
 Measurement range (Kcell=0.01) 0.00...1.999mg/l 0.005mg/l
 Measurement range (Kcell=0.1) 0.00...19.99mg/l 0.05mg/l
 Measurement range (Kcell=1) 0.0...199.9 mg/l 0.5 mg/l

200...1999 mg/l 1 mg/l
 2.00...19.99 g/l 0.01 g/l
 20.0...99.9 g/l 0.1 g/l
 Measurement range (Kcell=10) 100...999 g/l 1 g/l
 Accuracy (total dissolved solids) $\pm 0.5\% \pm 1\text{digit}$

Measurement of salinity
 Measurement range / Resolution 0.000...1.999g/l 1mg/l
 2.00...19.99g/l 10mg/l
 20.0...199.9g/l 0.1g/l
 Accuracy (salinity) $\pm 0.5\% \pm 1\text{digit}$

Automatic/manual temperature compensation
 0...100°C with α_t that can be selected from 0.00 to 4.00%/°C
Reference temperature 20°C o 25°C selectable from menu
 χ/TDS conversion factor 0.4...0.8
Cell constant K (cm⁻¹) 0.01 - 0.1 - 0.7 - 1.0 - 10.0

Standard solutions automatically detected (@25°C)
 147 $\mu\text{S/cm}$
 1413 $\mu\text{S/cm}$
 12880 $\mu\text{S/cm}$
 111800 $\mu\text{S/cm}$

Measurement of temperature by Instrument
 Pt100 measurement range -50...+200°C
 Pt1000 measurement range -50...+200°C
 Resolution 0.1°C
 Accuracy $\pm 0.25^\circ\text{C}$
 Drift after 1 year 0.1°C/year

(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:

K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹	
Conductivity ($\mu\text{S/cm}$)	Resistivity (M $\Omega\cdot\text{cm}$)	Conductivity ($\mu\text{S/cm}$)	Resistivity(M $\Omega\cdot\text{cm}$)
0.001 $\mu\text{S/cm}$	1000 M $\Omega\cdot\text{cm}$	0.01 $\mu\text{S/cm}$	100 M $\Omega\cdot\text{cm}$
0.002 $\mu\text{S/cm}$	500 M $\Omega\cdot\text{cm}$	0.02 $\mu\text{S/cm}$	50 M $\Omega\cdot\text{cm}$
0.003 $\mu\text{S/cm}$	333 M $\Omega\cdot\text{cm}$	0.03 $\mu\text{S/cm}$	33 M $\Omega\cdot\text{cm}$
0.004 $\mu\text{S/cm}$	250 M $\Omega\cdot\text{cm}$	0.04 $\mu\text{S/cm}$	25 M $\Omega\cdot\text{cm}$
...

ORDERING CODES

HD3456.2: The kit is composed of: instrument HD3456.2 **datalogger**, for the measurement of pH - redox - conductivity - resistivity - TDS - salinity - temperature, 3 1.5V alkaline batteries, operating manual and **DeltaLog9 version 2.0**.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.



pH



χ



Ω



TDS

ACCESSORIES

HD2110CSNM: 8-pole connection cable Mini Din - Sub D 9-pole female for RS232C, for connection to PC without USB input.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole Mini Din for connection to PC with USB input.

SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

pH Electrodes

KP20: Combined pH electrode for common use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for common use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. electrolyte, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for common use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled with screw connector S7, body in glass.

KP 100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

ORP Electrodes

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

Electrode characteristics at page 402

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for refilling of the electrodes.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Combined conductivity and temperature probes

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant K = 0.7. Measurement range 5µS/cm ...200mS/cm, 0...90°C.

SPT401.001: Combined conductivity and temperature 2-electrode cell in stainless steel AISI 316. Cell constant K = 0.01. Measurement range 0.04µS/cm ...20µS/cm, 0...120°C. Measurement in closed-cell..

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 0.1. Measurement range 0.1µS/cm ...500µS/cm, 0...80°C.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 1. Measurement range 10µS/cm ...10mS/cm, 0...80°C.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 10. Measurement range 500µS/cm ...200mS/cm, 0...80°C.

Electrode dimensions and characteristics at page 402

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147µS/cm @25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413µS/cm @25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880µS/cm @25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800µS/cm @25°C - 200cc.

Temperature probes complete with TP47 module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2 wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.





HD 2256.2 BENCH-TOP CONDUCTIVITY AND pH METER

The **HD2256.2** is a bench top instrument for electrochemical measures: **pH**, **conductivity** and **temperature**. It is fitted with a large backlit LCD display. The **HD2256.2** measures **pH**, **mV**, **redox potential** (ORP) with pH, redox electrodes or electrodes with separate reference. **Conductivity and resistivity** in liquids, **total dissolved solids** (TDS) and **salinity** with combined 4-ring and 2-ring conductivity/temperature probes. The conductivity probes can have a direct input or with SICRAM module. The inputs are separate.

The instruments is fitted with an input for the measurement of **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers.

- The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers Temperature compensation can be automatic or manual.
- The conductivity probe calibration can be performed automatically with automatically detected conductivity calibration solutions: 147µS/cm, 1413µS/cm, 12880µS/cm or 111800µS/cm or manually with calibration solutions having different values.
- Conductivity, dissolved oxygen and temperature probes fitted with SICRAM module can store factory and calibration data inside.

The instruments HD2256.2 is a **datalogger**, it can memorize up to 2,000 samples of data. The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing parameters can be configured using the menu. The RS232C serial port can be used to transfer the acquired measurements to a 24 column portable printer in real time (HD40.1 or HD40.2). The instruments equipped with **HD22BT** (Bluetooth) option can transfer data without any connection to a PC or printer fitted with Bluetooth input or through Bluetooth/RS232C converter. The software DeltaLog11 allows instrument management and configuration, and data processing on PC.

The instruments have IP66 protection degree.

Technical characteristics HD2256.2

pH - mV - χ - Ω - TDS - NaCl - °C - °F

Instrument

Dimensions (Length x Width x Height)	265x185x70mm
Weight	490g
Materials	ABS, rubber
Display	Back lighted, matrix point display. 240x64 points, visible area: 128x35mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensate

Protection degree

IP66

Power

Mains adapter (cod. SWD10)
12Vdc/1A

Auxiliary socket

For supplying of electrode holder with built-in stirrer HD22.2

Security of memorized data

Unlimited


Time

Date and hour

Real time schedule with backup battery
3.6V - ½AA

Accuracy

1min/month max drift

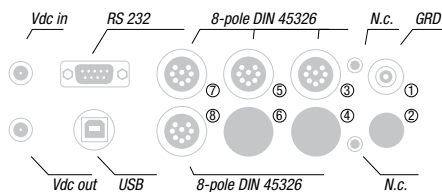

Measured values storing		Resolution																													
Quantity	2000 screens	100k...999kΩ-cm	1kΩ-cm																												
Storage interval	1s ... 999s	1...10MΩ-cm	1MΩ-cm																												
Calibration storage		Measuring range (Kcell=10)	0.5...5.0Ω-cm																												
Quantity	Last 8 calibrations of each physical quantity	Accuracy (resistivity)	±0.5% ±1digit																												
RS232C serial interface		Measurement of total dissolved solids (with coefficient $\chi/TDS=0.5$)																													
Type	RS232C electrically isolated	Measuring range (Kcell=0.01)	0.00...1.999mg/l 0.005mg/l																												
Baud rate	Can be set from 1200 to 115200 baud	Measuring range (Kcell=0.1)	0.00...19.99mg/l 0.05mg/l																												
Data bit	8	Measuring range (K cell=1)	0.0...199.9 mg/l 0.5 mg/l																												
Parity	None		200...1999 mg/l 1 mg/l																												
Stop bit	1		2.00...19.99 g/l 0.01 g/l																												
Flow Control	Xon/Xoff		20.0...199.9 g/l 0.1 g/l																												
Length of serial cable	Max 15m	Measuring range (Kcell=10)	100...999 g/l 1 g/l																												
USB Interface		Accuracy (total dissolved solids)	±0.5% ±1digit																												
Type	1.1 - 2.0 electrically isolated	Measurement of salinity by instrument																													
USB Interface	optional	Measuring range	0.000...1.999g/l 1mg/l																												
Connections			2.00...19.99g/l 10mg/l																												
Input for temperature probes with SICRAM modules⑤	8-pole male DIN45326 connector		20.0...199.9 g/l 0.1 g/l																												
pH/mV input ①	BNC female	Accuracy (salinity)	±0.5% ±1digit																												
Input for SICRAM module	8-pole male DIN45326 connector	Automatic/manual temperature compensation																													
pH/ temperature ③			0...100°C with $\alpha_T = 0.00...4.00\%/^{\circ}\text{C}$																												
2/ 4- electrode direct conductivity input ⑧	8-pole male DIN45326 connector	Reference temperature	0...50°C																												
Input conductivity electrodes with SICRAM module⑦	8-pole male DIN45326 connector	Conversion factor χ/TDS	0.4...0.8																												
Serial interface	DB9 connector (9- pole male)	Cell constant K (cm ⁻¹) already set on instrument	0.01 - 0.1 - 0.5 - 0.7 - 1.0 - 10.0																												
USB interface	USB connector type B	Cell constants K(cm ⁻¹) that can be set by user	0.01...20.00																												
Bluetooth	Optional	Standard solutions automatically detected (@25°C)																													
Mains adapter	2-pole connector (Ø5.5mm-2.1mm). Positive at centre		147µS/cm																												
Outlet for power supply of electrode holder with built-in magnetic stirrer	2-pole connector (Ø5.5mm-2.1mm). Positive at centre (output 12Vdc/200mA max).		1413µS/cm																												
pH measurement by instrument			12880µS/cm																												
Measuring range	-9.999...+19.999pH		111800µS/cm																												
Resolution	0.01 o 0.001pH selectable from menu	Measurement of temperature by instrument																													
Accuracy	±0.001pH ±1digit	Pt100 measuring range	-50...+150°C																												
Input impedance	>10 ¹² Ω	Pt1000 measuring range	-50...+150°C																												
Calibration error @25°C	Offset! > 20mV	Resolution	0.1°C																												
	Slope > 63mV/pH o Slope < 50mV/pH	Accuracy	±0.1°C ±1digit																												
	Sensitivity > 106.5% or Sensitivity < 85%	Drift after 1 year	0.1°C/year																												
Calibration points	Up to 5 points with 13 automatically detected buffer solutions	(*) The resistivity measurement is obtained from the reciprocal of conductivity measurement. Close to the bottom of the scale, the indication of resistivity appears like reported in the table below:																													
Standard solutions automatically detected (@25°C)	1.679pH - 2.000pH - 4.000pH - 4.008pH 4.010pH - 6.860pH - 6.865pH - 7.000pH 7.413pH - 7.648pH - 9.180pH - 9.210pH 10.010pH	<table> <tr> <th colspan="2">K cell = 0.01 cm⁻¹</th><th colspan="2">K cell = 0.1 cm⁻¹</th></tr> <tr> <th>Conductivity (µS/cm)</th><th>Resistivity (MΩ-cm)</th><th>Conductivity (µS/cm)</th><th>Resistivity(MΩ-cm)</th></tr> <tr> <td>0.001 µS/cm</td><td>1000 MΩ-cm</td><td>0.01 µS/cm</td><td>100 MΩ-cm</td></tr> <tr> <td>0.002 µS/cm</td><td>500 MΩ-cm</td><td>0.02 µS/cm</td><td>50 MΩ-cm</td></tr> <tr> <td>0.003 µS/cm</td><td>333 MΩ-cm</td><td>0.03 µS/cm</td><td>33 MΩ-cm</td></tr> <tr> <td>0.004 µS/cm</td><td>250 MΩ-cm</td><td>0.04 µS/cm</td><td>25 MΩ-cm</td></tr> <tr> <td>...</td><td>...</td><td>...</td><td>...</td></tr> </table>		K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹		Conductivity (µS/cm)	Resistivity (MΩ-cm)	Conductivity (µS/cm)	Resistivity(MΩ-cm)	0.001 µS/cm	1000 MΩ-cm	0.01 µS/cm	100 MΩ-cm	0.002 µS/cm	500 MΩ-cm	0.02 µS/cm	50 MΩ-cm	0.003 µS/cm	333 MΩ-cm	0.03 µS/cm	33 MΩ-cm	0.004 µS/cm	250 MΩ-cm	0.04 µS/cm	25 MΩ-cm
K cell = 0.01 cm ⁻¹		K cell = 0.1 cm ⁻¹																													
Conductivity (µS/cm)	Resistivity (MΩ-cm)	Conductivity (µS/cm)	Resistivity(MΩ-cm)																												
0.001 µS/cm	1000 MΩ-cm	0.01 µS/cm	100 MΩ-cm																												
0.002 µS/cm	500 MΩ-cm	0.02 µS/cm	50 MΩ-cm																												
0.003 µS/cm	333 MΩ-cm	0.03 µS/cm	33 MΩ-cm																												
0.004 µS/cm	250 MΩ-cm	0.04 µS/cm	25 MΩ-cm																												
...																												
mV measurement by instrument		ORDERING CODES																													
Measuring range	-1999.9...+1999.9mV	HD2256.2: The kit is composed of: instrument HD2256.2 for the measurement of pH - redox - conductivity - resistivity - TDS - salinity - temperature, datalogger , stabilized power supply at mains voltage 100-240Vac/12Vdc-1A., instructions manual and software DeltaLog11.																													
Resolution	0.1mV	pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.																													
Accuracy	±0.1mV ±1digit	ACCESSORIES																													
Drift after 1 year	0.5mV/year	9CPRS232: Connection cable SubD female 9- pole for serial output RS232C.																													
Conductivity measurement by instrument		CP22: USB 2.0 connection cable - connector typo A - connector type B.																													
Measuring range (Kcell=0.01)	0.000...1.999µS/cm	DeltaLog11: Software for download and management of the data on PC using Windows 98 to Vista operating systems.																													
Measuring range (Kcell=0.1)	0.00...19.99µS/cm	SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.																													
Measuring range (K cell=1)	0.0...199.9µS/cm	HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.																													
	200...1999µS/cm	HD40.2: 24-column portable thermal printer, Bluetooth and serial interface , 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (optional) or the cable HD 2110 CSNM (optional).																													
	2.00...19.99mS/cm	HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).																													
	20.0...199.9mS/cm																														
Measuring range (Kcell=10)	200...1999mS/cm																														
Accuracy (conductivity)	±0.5% ±1digit																														
Measurement of resistivity by instrument																															
Measuring range (Kcell=0.01)	Up to 1GΩ-cm (*)																														
Measuring range (Kcell=0.1)	Up to 100MΩ-cm (*)																														
Measuring range (K cell=1)	5.0...199.9Ω-cm 0.1Ω-cm																														
	200...999Ω-cm 1Ω-cm																														
	1.00k...19.99kΩ-cm 0.01kΩ-cm																														
	20.0k...99.9kΩ-cm 0.1kΩ-cm																														

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

HD22BT: Bluetooth module for wireless data transmission from instrument to PC. **The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.**

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

pH electrodes without SICRAM module (Inputs ① and ②)

KP20: Combined pH electrode for general use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for general use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. Liquid reference filling, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for general use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled, with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled, with screw connector S7, body in glass.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

ORP Electrodes (inputs ① and ②)

KP 90: REDOX PLATINUM liquid filled electrode with S7 screw connector, glass body.

KP 91: Gel REDOX PLATINUM electrode, 1m cable with BNC, EPOXY body

Characteristics and dimensions of the probes at page 397

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

pH electrodes with SICRAM module (Input ③)

KP63TS: Combined pH/temperature electrode with SICRAM module, body in Epoxy, Ag/AgCl sat KCl.

SICRAM Module with BNC input for pH electrodes (Input ③)

KP47: SICRAM module for pH electrode with BNC standard connector.

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for electrode refilling.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Conductivity probes and combined conductivity and temperature probes without SICRAM module (Input ⑦)

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant K = 0.7. Measurement range 5µS/cm ...200mS/cm, 0...90°C.

SPT401.001: Combined conductivity and temperature 2- electrode cell in stainless steel AISI 316. Cell constant K = 0.01. Measurement range 0.04µS/cm ...20µS/cm, 0...120°C. Measurement in closed-cell.

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 0.1. Measurement range 0.1µS/cm ...500µS/cm, 0...80°C.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 1. Measurement range 10µS/cm ...10mS/cm, 0...80°C.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 10. Measurement range 500µS/cm ...200mS/cm, 0...80°C.

Combined conductivity / temperature probes with SICRAM module (Input ⑧)

SPT1GS: Combined conductivity /temperature 2-electrode Platinum- wire cell, body in glass with SICRAM module. Cell constant K = 1. Measuring range 10µS/cm ...10mS/cm, 0...80°C.

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147µS/cm @25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413µS/cm @25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880µS/cm @25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800µS/cm @25°C - 200cc.

Temperature probes complete with SICRAM module (Input ⑤)

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 metre.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47 module (input⑤)

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



μ



mV



HD 3409.2 BENCH-TOP DISSOLVED OXYGEN METER

The **HD3409.2** is a bench top instrument for electrochemical measures: **dissolved oxygen** and **temperature**.

The displayed data can be stored (**datalogger**) and can be transferred to PC or serial printer thanks to the multi-standard serial ports RS232C and USB2.0 and software DeltaLog9 (Vers.2.0 and subsequent ones). The storing and printing parameters can be set from menu.

The **HD3409.2** measures the **concentration** (in mg/l) of **dissolved Oxygen in liquids**, the **saturation index** (in %) and the **temperature** using SICRAM combined probes of polarographic type with two or three electrodes and integrated temperature sensor. **Temperature** is measured by Pt100-SICRAM or direct 4 wire-immersion, penetration or contact probes.

Thanks to an internal pressure sensor, the instruments automatically compensate for barometric pressure. The instrument anticipates automatic compensation of the Oxygen probe membrane permeability and of the salinity of the liquid being examined. The dissolved Oxygen probe's quick calibration function guarantees timely correctness of the performed measurements.



The display shows continually the temperature in °C or °F and one selectable parameter according to the connected probe type. Printing and storage always include the temperature in °C or °F and one selectable parameter for each probe type.

Other common function of this instrument series include: Max, Min and Avg function, the Auto-HOLD function, the automatic turning off which can also be excluded.

The instruments have IP66 protection degree.

Technical characteristics HD3409.2

mg/l O₂, %O₂, mbar, °C/°F measurement

Instrument

Dimensions (Length x Width x Height)	220x120x55mm
Weight	460g (complete with batteries)
Materials	ABS, rubber
Display	2x4½ characters plus symbols visible area: 52x42mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% RH without condensation
Protection degree	IP66

Power

Batteries	3 batteries 1.5V type AA
Autonomy (only batteries)	100 hours with 1800mAh alkaline batteries
Mains (cod. SWD10)	Output mains adapter 100-240Vac/ 12Vdc-1A

Security of memorized data

Unlimited

Selectable storage interval

1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

Time

Date and hour	Schedule in real time
Accuracy	1min/month max drift

Serial interface RS232C

Type	RS232C electrically isolated
Baud rate	Can be set from 1200 to 38400 baud
Data bit	8
Parity	None
Stop bit	1
Flow Control	Xon/Xoff
Serial cable length	Max 15m
Selectable print interval	immediate or 1s, 5s, 10s, 15s, 30s, 1min, 2min, 5min, 10min, 15min, 20min, 30min and 1hour

USB Interface


Type	1.1 - 2.0 electrically isolated
------	---------------------------------

Common connections to all models

Serial interface and USB	8-pole MiniDin connector
Mains adapter (cod. SWD10)	2-pole connector (positive at centre) 12Vdc/1A

Power absorbed with instrument off

Without dissolved oxygen probe	20µA
With dissolved oxygen probe	40µA

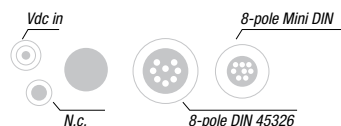

Storage of the measured values

Type	2000 pages of 9 samples each
Quantity	18,000 measures made up of the four parameters mg/l O ₂ , %O ₂ , mbar, [°C or °F]

Measurement connections

Input for Oxygen probes	8-pole male DIN45326 connector
Input for temperature probes with SICRAM module or TP47 module	8-pole male DIN45326 connector

Measurement of the concentration of dissolved Oxygen

Measurement range	0.00...90.00mg/l
Resolution	0.01mg/l
Accuracy	±0.03mg/l/±1digit 60...110%, 1013mbar, 20...25°C)

Measurement of the saturation index of dissolved Oxygen

Measurement range	0.0...600.0%
Resolution	0.1%
Accuracy	±0.3% ±1digit (in the range 0...199.9%) ±1% ±1digit (in the range 00.0...600.0%)

Automatic/manual temperature compensation

0...50°C

Measurement of barometric pressure

Measurement range	0.0...1100.0mbar
Resolution	0.1mbar
Accuracy	±2mbar±1digit between 18 and 25°C ±(2mbar+0.1mbar/°C) in the remaining range

Salinity setting

Setting range	0.0...70.0g/l
Resolution	0.1g/l

Temperature measurement with the sensor inside the dissolved Oxygen probe

Measurement range	0.0...+45.0°C
Resolution	0.1°C
Accuracy	±0.1°C
Drift after 1 year	0.1°C/year

Temperature measurement by Instrument with Pt100 probe

Pt100 Measurement range	-200...+650°C
Resolution	0.1°C
Accuracy	±0.1°C
Drift after 1 year	0.1°C/year

ORDERING CODES

HD3409.2: The kit is composed of: instrument HD3409.2 **data logger**, for the measurement of dissolved oxygen concentration - saturation index - temperature, calibrator HD9709/20, 3 1.5V alkaline batteries, operating manual and **DeltaLog9 version 2.0**.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

ACCESSORIES

HD2110CSNM: 8-pole connection cable Mini Din - Sub D 9-pole female for RS232C, for connection to PC without USB input.

HD2101/USB: Connection cable USB 2.0 connector type A - 8-pole Mini Din for connection to PC with USB input.

SWD10: Stabilized power supply at 120-240Vac/12Vdc/1A mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (**optional**) or supplier SWD10 (**optional**).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes to instrument series HD34..., without amplifying electronics and linearization.

Combined dissolved oxygen and temperature probes

D09709 SS: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 2m. Ø12mm x 120mm.

D09709 SS.5: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 5m. Ø12mm x 120mm.

Accessories

D09709 SSK: Accessory kit for the D09709 SS probe consisting of three membranes, 50ml of zero solution, 50ml of electrolyte solution.

D09709.20: Calibrator for polarographic probes D09709SS and D09709SS.5.

Probe dimensions and characteristics at page 403

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 m.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47 module

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



mg/l



%sat



mbar



°C



HD 2259.2 BENCH-TOP DISSOLVED OXYGEN AND pH METER

The **HD2259.2** a bench top instrument for electrochemical measures: **pH**, **dissolved oxygen**, and **temperature**. It is fitted with a large backlit LCD display. The **HD2259.2** measures **pH**, **mV**, **redox potential** (ORP) with pH, redox electrodes or electrodes with separate reference; the **concentration of dissolved oxygen** in liquids (in mg/l), and **saturation index** (in %), using SICRAM combined probes of polarographic type with two or three electrodes and integrated temperature sensor.

The instrument fitted with an input for the measurement of **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

- The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers Temperature compensation can be automatic or manual.
- The dissolved Oxygen probe's quick calibration function guarantees timely correctness of the performed measurements.
- Conductivity, dissolved oxygen and temperature probes fitted with SICRAM module can store factory and calibration data inside.

The instrument HD2259.2 is a **datalogger**, it can memorize up to 2,000 samples of data:

- pH or mV, concentration of dissolved oxygen or saturation index and saturation index and temperature:
- pH or mV, conductivity or resistivity or TDS or salinity, concentration of dissolved oxygen and temperature:

The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing parameters can be configured using the menu. The RS232C serial port can be used to transfer the acquired measurements to a 24 column portable printer in real time (S'print-BT).

The instruments equipped with **HD22BT** (Bluetooth) option can transfer data without any connection to a PC or printer fitted with Bluetooth input or through Bluetooth/RS232C converter. The software DeltaLog11 allows instrument management and configuration, and data processing on PC.

The instruments have IP66 protection degree.

Technical characteristics HD2259.2

pH - mV - mg/l O₂ - %O₂ - mbar - °C - °F measurement

Instrument

Dimensions (Length x Width x Height)	265x185x70mm
Weight	490g
Materials	ABS, rubber
Display	Back lighted, matrix point display. 240x64 points, visible area: 128x35mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensate
Protection degree	IP66

Power

Mains adapter (cod. SWD10)
12Vdc/1A

Auxiliary socket

For supplying of electrode holder with built-in stirrer HD22.2


Security of memorized data

Unlimited

Time

Date and hour

Real time schedule with backup battery E 3.6V - 1/2AA

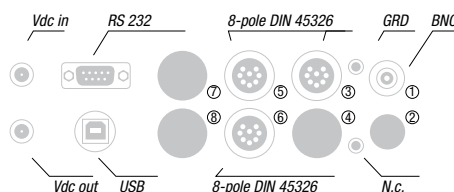

Accuracy	1min/month max drift	Automatic temperature compensation	0...50°C
<i>Measured values storing</i>			
Quantity	2000 screens	Measurement of barometric pressure	
Storage interval	1s ... 999s	Measuring range	0.0...1100.0mbar
		Resolution	0.1mbar
		Accuracy	±2mbar±1digit between 18 and 25°C ±(2mbar+0.1mbar/°C) in the remaining range
<i>Calibration storage</i>			
Quantity	Last 8 calibrations of each physical quantity	Salinity setting	
		Setting	directly from menu or automatically by conductivity measurement
		Setting range	0.0...70.0g/l
		Resolution	0.1g/l
<i>RS232C serial interface</i>			
Type	RS232C electrically isolated	Temperature measurement with the sensor inside the dissolved oxygen probe	
Baud rate	Can be set from 1200 to 115200 baud	Measuring range	0.0...50.0°C
Data bit	8	Resolution	0.1°C
Parity	None	Accuracy	±0.1°C
Stop bit	1	Drift after 1 year	0.1°C/year
Flow Control	Xon/Xoff		
Length of serial cable	Max 15m		
<i>USB Interface</i>			
Type	1.1 - 2.0 electrically isolated	Measurement of temperature by instrument	
Bluetooth Interface	optional	Pt100 measuring range	-50...+150°C
		Pt1000 measuring range	-50...+150°C
		Resolution	0.1°C
		Accuracy	±0.1°C ±1digit
		Drift after 1 year	0.1°C/year
<i>Connections</i>			
Input for temperature probes with SICRAM modules⑤	8-pole male DIN45326 connector	ORDERING CODES	
pH/mV inputs①	BNC female	HD2259.2: The kit is composed of: instrument HD2259.2 for the measurement of pH - redox - concentration of dissolved oxygen, saturation index - temperature, datalogger , stabilized power supply at mains voltage 100-240Vac/12Vdc-1A., calibrator HD9709/20, instructions manual and software DeltaLog11.	
Input SICRAM module	8-pole male DIN45326 connector	pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.	
pH/temperature probes③	8-pole male DIN45326 connector	ACCESSORIES	
Input dissolved oxygen ⑥	8-pole male DIN45326 connector	9CPRS232: Connection cable SubD female 9- pole for serial output RS232C.	
Serial interface	DB9 connector (9- pole male)	CP22: USB 2.0 connection cable - connector type A - connector type B.	
USB interface	USB connector type B	DeltaLog11: Software for download and management of the data on PC using Windows 98 to Vista operating systems.	
Bluetooth	Optional	SWD10: Stabilized power supply at 100-240Vac/12Vdc/1A mains voltage.	
Mains adapter	2-pole connector (Ø5.5mm-2.1mm). Positive at centre	HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.	
Outlet for power supply of electrode holder with built-in magnetic stirrer	2- pole connector (Ø5.5mm-2.1mm). Positive at centre (output 12Vdc/200mA max).	HD40.2: 24-column portable thermal printer, Bluetooth and serial interface , 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (optional) or the cable HD 2110 CSNM (optional).	
<i>Measurement of pH by instrument</i>			
Measuring range	-9.999...+19.999pH	HD2110CSP: Connection cable for instruments series HD34...to printer S'print-BT	
Resolution	0.01 o 0.001pH selectable from menu	HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).	
Accuracy	.001pH ±1digit	HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.	
Input impedance		HD22BT: Bluetooth module for wireless data transmission from instrument to PC. The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.	
Calibration error @25°C	Offset > 20mV Slope > 63mV/pH o Slope < 50mV/pH Sensitivity < 85% or sensitivity < 85% Up to 5 points with 13 automatically detected buffer solutions		
Calibration points	1.679pH - 2.000pH - 4.000pH - 4.008pH 4.010pH - 6.860pH - 6.865pH - 7.000pH 7.413pH - 7.648pH - 9.180pH - 9.210pH 10.010pH		
Automatically detected pH standard solutions (@25°C)			
<i>mV measurement by instrument</i>			
Measuring range	-1999.9...+1999.9mV		
Resolution	0.1mV		
Accuracy	±0.1mV ±1digit		
Drift after 1 year	0.5mV/year		
<i>Measurement of dissolved oxygen by instrument</i>			
Resolution	0.01mg/l		
Measuring range	0.00...90.00mg/l		
Accuracy	±0.03mg/l±1digit (60...110%, 1013mbar, 20...25°C)		



pH



mg/l

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

Accessories

pH electrodes without SICRAM module (Inputs ① and ②)

KP20: Combined pH electrode for general use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for general use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. Liquid reference filling, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for general use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled, with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled, with screw connector S7, body in glass.

KP100: Flat membrane gel combined pH electrode with S7 screw connector, glass body, for skin, leather, paper.

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

pH electrodes with SICRAM module (Input ③)

KP63TS: Combined pH/temperature electrode with SICRAM module, body in Epoxy, Ag/AgCl sat KCl.

ORP Electrodes (Inputs ① and ②)

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

SICRAM module with BNC input for pH electrodes (input ③)

KP47: Sicram module for pH electrode with standard BNC connector.

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for electrode refilling.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (tiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Combined dissolved oxygen/temperature probes (Input ⑥)

D09709 SS: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 2m. Ø12mm x 120mm.

D09709 SS.5: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 5m. Ø12mm x 120mm.

Accessories

D09709 SSK: Accessory kit for the D09709 SS probe consisting of three membranes, 50ml of zero solution, 50ml of electrolyte solution

D09709.20: Calibrator for polarographic probes D09709SS and D09709SS.5.

Temperature probes complete with SICRAM module (Input ⑤)

TP87: PT100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 metre.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 metres.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 metres.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 metres.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 metres.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 metres.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 metres.

Temperature probes complete with TP47 module (input ⑤)

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 metres.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 metres.

TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 metre.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 metre.

Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.





HD 22569.2 BENCH-TOP METER FOR pH - CONDUCTIVITY - DISSOLVED OXYGEN

The instrument **HD22569.2** is a bench top instrument for electrochemical measures: **pH**, **conductivity**, **dissolved oxygen**, and **temperature**. It is are fitted with a large backlighted LCD display.

The **HD22569.2** measures **pH**, **mV**, **redox potential** (ORP) with pH, redox electrodes or electrodes with separate reference; **conductivity**, **resistivity** in liquids, **total dissolved solids** (TDS) and **salinity** with combined 4-ring and 2-ring conductivity/temperature probes with direct input or SICRAM module; **concentration of dissolved oxygen** in liquids (in mg/l) and **saturation index** (in %), using SICRAM combined probes of polarographic type with two or three electrodes and integrated temperature sensor.

The instruments is fitted with an input for the measurement of **temperature** with Pt100 or Pt1000 immersion, penetration or contact probes. The temperature probes are equipped with an automatic recognition module and factory calibration data are stored inside.

- The pH electrode calibration can be carried out on one or five points and the calibration sequence can be chosen from a list of 13 buffers Temperature compensation can be automatic or manual.
- The conductivity probe calibration can be performed automatically with automatically detected conductivity calibration solutions: 147µS/cm, 1413µS/cm, 12880µS/cm or 111800µS/cm or manually with calibration solutions having different values.
- The dissolved Oxygen probe's quick calibration function guarantees timely correctness of the performed measurements.
- Conductivity, dissolved oxygen and temperature probes fitted with SICRAM module can store factory and calibration data inside.

The instruments HD22569.2 is a **datalogger**, it can memorize up to 2,000 samples of data:

- pH or mV, conductivity or resistivity or TDS or salinity, concentration of dissolved oxygen and temperature:

The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0. The storing parameters can be configured using the menu. The RS232C serial port can be used to transfer the acquired measurements to a 24 column portable printer in real time (HD40.1 or HD40.2).

The instruments equipped with **HD22BT** (Bluetooth) option can transfer data without any connection to a PC or printer fitted with Bluetooth input or through Bluetooth/RS232C converter. The software DeltaLog11 allows instrument management and configuration, and data processing on PC.

The instruments have IP66 protection degree.

Technical characteristics of HD22569.2

pH - mV - χ - Ω - TDS - NaCl - mg/l O₂ - %O₂ - mbar - °C - °F measurement

Instrument

Dimensions (Length x Width x Height)	265x185x70mm
Weight	490g
Materials	ABS, rubber
Display	Back lighted, matrix point display. 240x64 points, visible area: 128x35mm

Operating conditions

Working temperature	-5 ... 50°C
Storage temperature	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensate

Protection degree

IP66

Power

Mains adapter (cod. SWD10)
12Vdc/1A

Auxiliary socket

For supplying of electrode holder with built-in stirrer HD22.2

Security of memorized data

Unlimited

Time

Date and hour

Real time schedule with backup battery E
3.6V - ½AA


Accuracy

1min/month max drift

Measured values storing

Quantity	2000 screens
Storage interval	1s ... 999s

Calibration storage

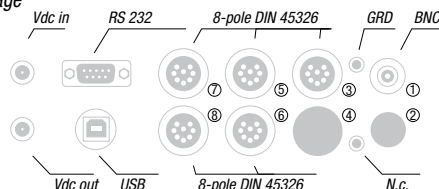

Quantity	Last 8 calibrations of each physical quantity	Measurement range (Kcell=1)	0.0...199.9 mg/l 200...1999 mg/l 2.00...19.99 g/l 20.0...99.9 g/l	Resolution 0.5 mg/l 1 mg/l 0.01 g/l 0.1 g/l
<i>RS232C serial interface</i>		Measurement range (Kcell=10)	100...999 g/l	1 g/l
Type	RS232C electrically isolated	Accuracy (total dissolved solids)	±0.5% ±1digit	
Baud rate	Can be set from 1200 to 115200 baud	<i>Measurement of salinity</i>		
Data bit	8	Measurement range	0.000...1.999g/l 2.00...19.99g/l 20.0...199.9g/l	1mg/l 10mg/l 0.1g/l
Parity	None	Accuracy (salinity)	±0.5% ±1digit	
Stop bit	1	<i>Automatic/manual temperature compensation</i>	0...100°C with $\alpha_T = 0.00...4.00\%/^{\circ}\text{C}$	
Flow Control	Xon/Xoff	<i>Reference temperature</i>	0...50°C	
Length of serial cable	Max 15m	<i>Conversion factor χ/TDS</i>	0.4...0.8	
<i>USB Interface</i>		<i>Cell constants K (cm⁻¹)</i>	0.01 - 0.1 - 0.5 - 0.7 - 1.0 - 10.0	
Type	1.1 - 2.0 electrically isolated	<i>already set on instrument</i>		
<i>USB Interface</i>	optional	Cell constants K(cm ⁻¹) that can be set by user	0.01...20.00	
<i>Connections</i>		<i>Standard solutions automatically detected (@25°C)</i>		
Input for temperature probes with SICRAM modules⑤	8-pole male DIN45326 connector		147µS/cm 1413µS/cm 12880µS/cm 111800µS/cm	
pH/mV ① input	BNC female	<i>Measurement of concentration of dissolved oxygen by instrument</i>		
Input for SICRAM module	8-pole male DIN45326 connector	Measuring range	0.00...90.00mg/l	
pH/ temperature ③		Resolution	0.01mg/l	
2/ 4- electrode direct conductivity input ⑧	8-pole male DIN45326 connector	Accuracy	±0.03mg/l±1digit (60...110%, 1013mbar, 20...25°C)	
Conductivity SICRAM module input ⑦	8-pole male DIN45326 connector	<i>Measurement of saturation index of dissolved oxygen</i>		
Dissolved Oxygen input ⑥	8-pole male DIN45326 connector	Measuring range	0.0...600.0%	
Serial interface	DB9 connector (9- pole male)	Resolution	0.1%	
USB interface	USB connector type B	Accuracy	±0.3% ±1digit (in the range 0.0...199.9%) ±1% ±1digit (in the range 200.0...600.0%)	
Bluetooth	Optional	<i>Measurement of barometric pressure</i>		
Mains adapter	2- pole connector (Ø5.5mm-2.1mm). Positive at centre	Measuring range	0.0...1100.0mbar	
Outlet for power supply of electrode holder with built-in magnetic stirrer	2-pole connector (Ø5.5mm-2.1mm). Positive at centre (output 12Vdc/200mA max).	Resolution	0.1mbar	
		Accuracy	±2mbar±1digit between 18 and 25°C ±(2mbar+0.1mbar/°C) in the remaining range	
<i>pH measurement by instrument</i>		<i>Salinity setting</i>		
Measuring range	-9.999...+19.999pH	Setting	directly from menu or automatically by conductivity measurement	
Resolution	0.01 o 0.001pH selectable from menu	Setting range	0.0...70.0g/l	
Accuracy	±0.001pH ±1digit	Resolution	0.1g/l	
Input impedance	>10 ¹² Ω	<i>Temperature measurement with the sensor inside the dissolved Oxygen probe</i>		
Calibration error @25°C	Offset! > 20mV Slope > 63mV/pH o Slope < 50mV/pH Sensitivity > 106.5% or Sensitivity < 85%	Measurement range	0.0...+50.00°C	
Calibration points	Up to 5 points with 13 automatically detected buffer solutions	Resolution	0.1°C	
Automatically detected pH standard solutions (@25°C)	1.679pH - 2.000pH - 4.000pH - 4.008pH - 4.010pH 6.860pH - 6.865pH - 7.000pH - 7.413pH - 7.648pH 9.180pH - 9.210pH - 10.010pH	Accuracy	±0.1°C	
		Drift after 1 year	0.1°C/year	
<i>mV measurement by instrument</i>		<i>Automatic temperature compensation</i>	0...50°C	
Measuring range	-1999.9...+1999.9mV	<i>Measurement of temperature by instrument</i>		
Resolution	0.1mV	Pt100 measuring range	-50...+150°C	
Accuracy	±0.1mV ±1digit	Pt1000 measuring range	-50...+150°C	
Drift after 1 year	0.5mV/year	Resolution	0.1°C	
		Accuracy	±0.1°C ±1digit	
<i>Measurement of conductivity by instrument</i>		Drift after 1 year	0.1°C/year	
Measuring range (Kcell=0.01)	0.000...1.999µS/cm			
Measuring range (Kcell=0.1)	0.00...19.99µS/cm			
Measuring range (K cell=1)	0.0...199.9µS/cm			
	200...1999µS/cm			
	2.00...19.99mS/cm			
	20.0...199.9mS/cm			
Measuring range (Kcell=10)	200...1999mS/cm			
Accuracy (conductivity)	±0.5% ±1digit			
<i>Measurement of resistivity by instrument</i>				
Measuring range (Kcell=0.01)	Up to 1GΩ·cm (*)			
Measuring range (Kcell=0.1)	Up to 100MΩ·cm (*)			
Measuring range (K cell=1)	5.0...199.9Ω·cm			
	200...999Ω·cm			
	1.00k...19.99kΩ·cm			
	20.0k...99.9kΩ·cm			
	100k...999kΩ·cm			
	1...10MΩ·cm			
Measuring range (Kcell=10)	0.5...5.0Ω·cm			
Accuracy (resistivity)	±0.5% ±1digit			
<i>Measurement of total dissolved solids (with coefficient χ/TDS=0.5)</i>				
Measurement range (Kcell=0.01)	0.00...1.999mg/l			
Measurement range (Kcell=0.1)	0.00...19.99mg/l			

ORDERING CODES

HD22569.2: The kit is composed of: instrument HD22569.2 for the measurement of pH - redox - conductivity - resistivity - TDS - salinity - concentration of dissolved oxygen, saturation index - temperature, **datalogger**, stabilized power supply at mains voltage 100-240Vac/12Vdc-1A., calibrator HD9709/20, instructions manual and software DeltaLog11.

pH/mV electrodes, conductivity probes, dissolved oxygen probes, temperature probes, standard reference solutions for different measurement types, connection cables for pH electrodes with S7 connector, cables for data download to PC or printer have to be ordered separately.

Accessories

9CPRS232: Connection cable SubD female 9- pole for serial output RS232C.

CP225: USB 2.0 connection cable - connector type A - connector type B.

DeltaLog11: Software for download and management of the data on PC using Windows 98 to Vista operating systems.

SWD10: Stabilized power supply at 100-240Vac/12Vdc-1A mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

HD40.2: 24-column portable thermal printer, **Bluetooth and serial interface**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls. Requires the module HD22BT (optional) or the cable HD 2110 CSNM (optional).

HD22.2: Laboratory electrode holder composed of basis plate with incorporated magnetic stirrer, staff and replaceable electrode holder. Height max. 380mm. Powered by bench-top meters of the series HD22... with cable HD22.2.1 (optional) or supplier SWD10 (optional).

HD22.3: Laboratory electrode holder with metal basis plate. Flexible electrode holder for free positioning. For Ø 12mm probes.

HD22BT: Bluetooth module for wireless data transmission from instrument to PC. **The fitting of the module into the instrument is made exclusively by Delta Ohm, at the time of placing the order.**

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.

pH electrodes without SICRAM module (Inputs ① and ②)

KP20: Combined pH electrode for general use, gel filled with screw connector S7 body in Epoxy.

KP30: Combined pH electrode for general use, cable 1 m, gel filled, body in Epoxy.

KP50: Combined pH electrode with Teflon collar diaphragm, for emulsions, deionised water, S7 screw connector, gel filled, body in glass.

KP 61: Combined pH electrode, 3 diaphragms for milk, cream, etc. Liquid reference filling, with screw connector S7, body in glass.

KP 62: Combined pH electrode, 1 diaphragm for pure water, paints, etc. gel-filled, with screw connector S7, body in glass.

KP 63: Combined pH electrode for general use, varnish, cable 1 m, electrolyte KCl 3M body in glass.

KP 64: Combined pH electrode for water, varnish, emulsions, etc., electrolyte KCl 3M with screw connector S7, body in glass.

KP 70: Combined pH micro electrode diam. 4.5 x L=25 mm. Gel filled, with screw connector, body in glass.

KP 80: Combined pointed pH electrode, gel filled, with screw connector S7, body in glass.

CP: Extension cable 1.5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CP5: Extension cable 5m with BNC connectors on one side and S7 on the other side for electrode with S7 connector.

CE: S7 screw connector for pH electrode.

BNC: Female BNC for electrode extension.

pH electrodes with SICRAM module (Input ③)

KP63TS: Combined pH/temperature electrode with SICRAM module, body in Epoxy, Ag/AgCl sat KCl.

SICRAM Module with BNC input for pH electrodes (Input ③)

KP47: SICRAM module for pH electrode with BNC standard connector.

ORP Electrodes (Inputs ① and ②)

KP90: Redox Platinum electrode, with screw connector S7, electrolyte KCl 3M, body in glass.

KP91: Redox Platinum electrode with 1m cable, GEL filled, body in glass.

pH buffer solutions

HD8642: Buffer solution 4.01pH - 200cc.

HD8672: Buffer solution 6.86pH - 200cc.

HD8692: Buffer solution 9.18pH - 200cc.

Redox buffer solutions

HDR220: Redox buffer solution 220mV 0,5 l.

HDR468: Redox buffer solution 468mV 0,5 l.

Electrolyte solutions

KCL 3M: 50cc ready for use solution for electrode refilling.

Cleaning and maintenance

HD62PT: Diaphragm cleaning (thiourea in HCl) - 500ml.

HD62PP: Protein cleaning (pepsin in HCl) - 500ml.

HD62RF: Regeneration (fluorhydric acid) - 100ml.

HD62SC: Solution for electrode preservation - 500ml.

Conductivity probes and combined conductivity and temperature probes without SICRAM module (Input ②)

SP06T: Combined conductivity and temperature 4-electrode cell in Platinum, body in Pocan. Cell constant K = 0.7. Measurement range 5µS/cm ...200mS/cm, 0...90°C.

SPT401.001: Combined conductivity and temperature 2- electrode cell in stainless steel AISI 316. Cell constant K = 0.01. Measurement range 0.04µS/cm ...200µS/cm, 0...120°C. Measurement in closed-cell.

SPT01G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 0.1. Measurement range 0.1µS/cm ...500µS/cm, 0...80°C.

SPT1G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 1. Measurement range 10µS/cm ...10mS/cm, 0...80°C.

SPT10G: Combined conductivity and temperature 2-electrode Platinum-wire cell, body in glass. Cell constant K = 10. Measurement range 500µS/cm ...200mS/cm, 0...80°C.

Combined conductivity / temperature probes with SICRAM module (Input ③)

SPT1GS: Combined conductivity /temperature 2-electrode Platinum- wire cell, body in glass with SICRAM module. Cell constant K = 1. Measuring range 10µS/cm ...10mS/cm, 0...80°C.

Standard conductivity calibration solutions

HD8747: Standard calibration solution 0.001mol/l equal to 147µS/cm @25°C - 200cc.

HD8714: Standard calibration solution 0.01mol/l equal to 1413µS/cm @25°C - 200cc.

HD8712: Standard calibration solution 0.1mol/l equal to 12880µS/cm @25°C - 200cc.

HD87111: Standard calibration solution 1mol/l equal to 111800µS/cm @25°C - 200cc.

Combined dissolved oxygen/temperature probes (Input ⑥)

D09709 SS: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 2m. Ø12mm x 120mm.

D09709 SS.5: The kit includes: combined probe for measurement of O₂ and temperature with replaceable membrane, three membranes, 50ml of zero solution, 50ml of electrolyte solution. Cable length 5m. Ø12mm x 120mm.

Electrode dimensions and characteristics at page 403

Accessories

D09709 SSK: Accessory kit for the D09709 SS probe consisting of three membranes, 50ml of zero solution, 50ml of electrolyte solution

D09709.20: Calibrator for polarographic probes D09709SS and D09709SS.5.

Temperature probes complete with SICRAM module (Input ⑤)

TP87: Pt100 sensor immersion probe. Stem Ø 3 mm, length 70 mm. Cable length 1 metre.

TP4721.0: Pt100 sensor immersion probe. Stem Ø 3 mm, length 230 mm. Cable length 2 m.

TP473P.0: Pt100 sensor penetration probe. Stem Ø 4mm, length 150 mm. Cable length 2 m.

TP474C.0: Pt100 sensor contact probe. Stem Ø 4mm, length 230mm, contact surface Ø 5mm. Cable length 2 m.

TP475A.0: Air probe, sensor Pt100. Stem Ø 4mm, length 230mm. Cable length 2 m.

TP4721.5: Immersion probe, sensor Pt100. Stem Ø 6mm, length 500 mm. Cable length 2 m.

TP4721.10: Immersion probe, sensor Pt100. Stem Ø 6mm, length 1,000mm. Cable length 2 m.

Temperature probes complete with TP47 module (input ⑤)

TP47.100: Direct 4 wires Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 4 wires with connector, length 2 m.

TP47.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 230mm. Connection cable 2 wires with connector, length 2 m.











TP87.100: Pt100 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 4 wire connection cable with connector, length 1 m.

TP87.1000: Pt1000 sensor immersion probe. Probe's stem Ø 3mm, length 70mm. 2-wire connection cable with connector, length 1 m.



Accessories

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



Technical data of pH electrodes without SICRAM module

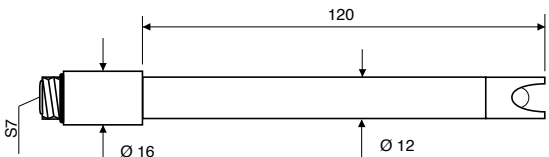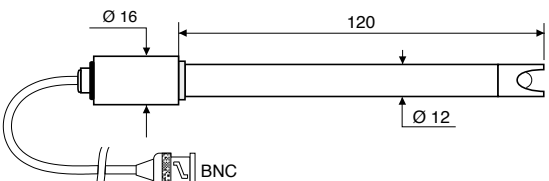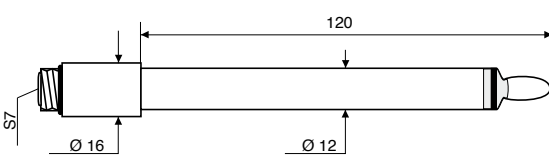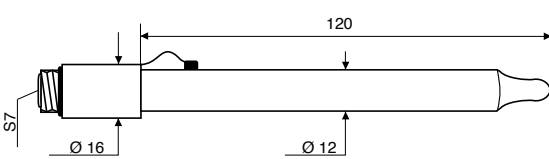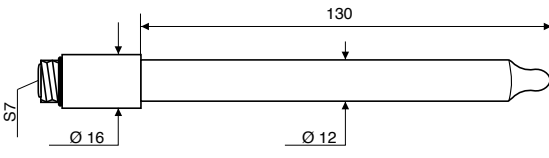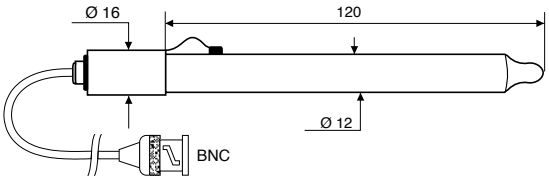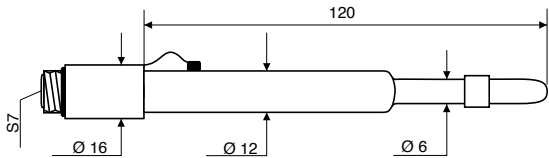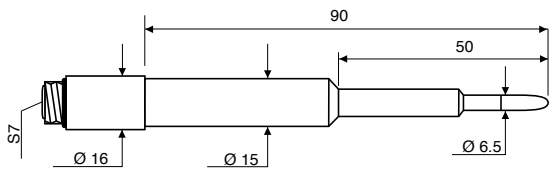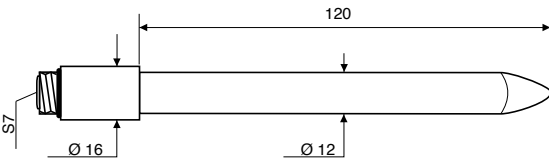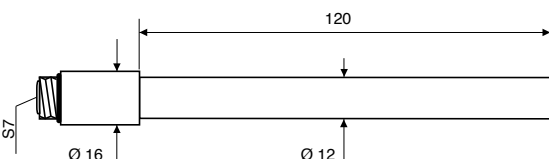ORDERING CODE	MEASUREMENT RANGE AND USE	DIMENSIONS
KP20	0...14pH / 0...80°C / 3bar Body in Epoxy - GEL filled 1 ceramic diaphragm Waste water, drinking water, paints, water emulsions, galvanic baths, fruit juices, water suspensions, titration, varnishes.	
KP30	0...14pH / 0...80°C / 3bar Body in Epoxy - GEL filled 1 ceramic diaphragm Cable L=1m with BNC Waste water, drinking water, water emulsions, galvanic baths, paints, varnishes, water suspensions, fruit juices, titration.	
KP50	0...14pH / 0...80°C / 3bar Body in glass - GEL filled 1 Teflon ring diaphragm Varnishes, cosmetics, water emulsions, galvanic baths, creams, deionised water, TRIS solutions, drinking water, fruit juices, low-ion-content solutions, mayonnaise, preserved food, paints, titration, titration in non-water solutions, water suspensions, detergents, waste water, viscous samples.	
KP61	2...14pH / 0...80°C / 3bar Body in glass Liquid reference filling Triple ceramic diaphragm Waste water, paste, bread, fruit juices, varnishes, cosmetics, creams, deionised water, drinking water, water emulsions, galvanic baths, detergents, yoghurt, milk, titration, preserved food, titration in non-water solutions, water suspensions, mayonnaise, wine, low ion-content solution, butter, proteic substances, paints, viscous samples	
KP62	0...14pH / 0...80°C / 3bar Body in glass - GEL filled 1 ceramic diaphragm Paints, varnishes, drinking water, water emulsions, fruit juices, galvanic baths, water suspensions, titration, waste water.	
KP63	0...14pH / 0...80°C / 1bar Body in glass Reference filling solution KCl 3M 1 ceramic diaphragm Cable L=1m with BNC Paints, varnishes, drinking water, water solutions, fruit juices, galvanic baths, water suspensions, titrations, waste water.	
KP64	0...14pH / 0...80°C / 0.1bar Body in glass Liquid reference KCl 3M Teflon collar diaphragm Paints, varnishes, cosmetics, creams, deionised water, drinking water, water emulsions, fruit juices, detergents, low ion-content solutions, preserved food, water suspensions, titration, titration in non-water solutions, TRIS solutions, waste water, viscous samples, wine.	
KP70	2...14pH / 0...50°C / 0.1bar Body in Epoxy - GEL filled 1 open junction Paste, bread, paints, varnishes, cosmetics, creams, drinking water, water emulsions, fruit juices, galvanic baths, detergents, mayonnaise, preserved foods, cheese, milk, water suspensions, viscous samples, waste water, butter, yoghurt.	
KP80	2...14pH / 0...60°C / 1bar Body in glass - GEL filled 1 open junction Paste, bread, paints, varnishes, cosmetics, creams, drinking water, water emulsions, fruit juices, galvanic baths, detergents, mayonnaise, preserved food, water suspensions, titration, titration in non-water solutions, viscous samples, waste water, yoghurt, milk, butter.	
KP100	2...14pH / 0...80°C / 1bar Body in glass Liquid reference KCl 3M Teflon ring diaphragm Flat membrane gel combined pH electrode, S7 connector, for skin, leather, paper.	




pH electrodes

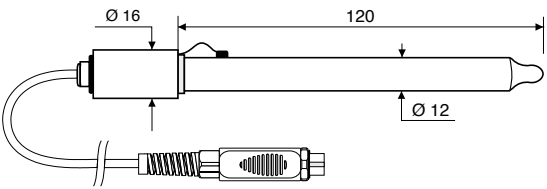ORDERING CODE	MEASUREMENT RANGE AND USE	DIMENSIONS
KP63TS	0...14pH / 0...80°C / 1bar Pt100 sensor Body in glass Reference filling solution KCl 3M 1 ceramic diaphragm Cable L=1m with SICRAM module Paints, varnishes, drinking water, water solutions, fruit juices, galvanic baths, water suspensions, titrations, waste water.	
KP47	Please refer to employed electrode.	



Redox Electrodes without SICRAM module

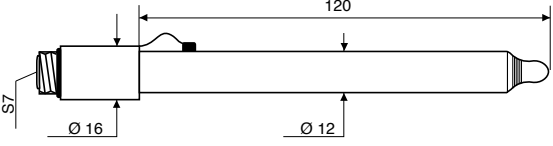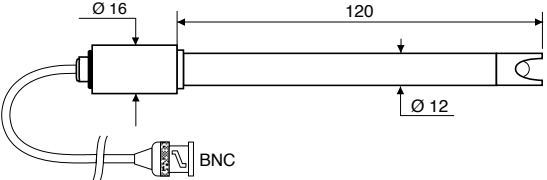ORDERING CODE	MEASUREMENT RANGE AND USE	DIMENSIONS
KP90	±2000mV 0...80°C 5bar Body in glass Reference filling solution KCl 3M General use	
KP91	±1000mV 0...60°C 1bar Body in Epoxy - GEL Cable L=1m with BNC General use No heavy tasks	


Combined 2-ring or 4-ring conductivity probes without SICRAM module

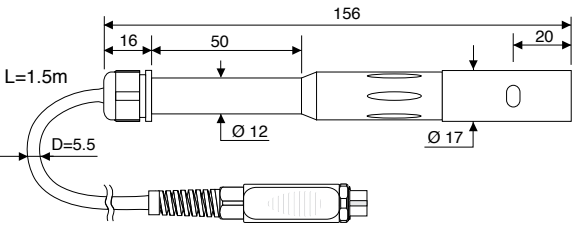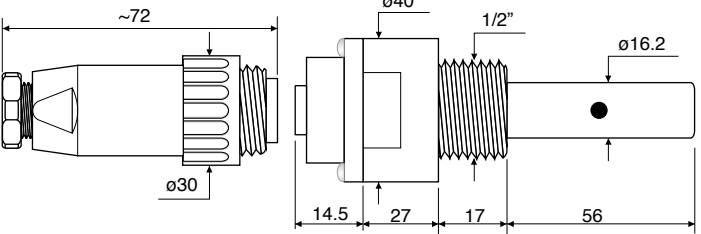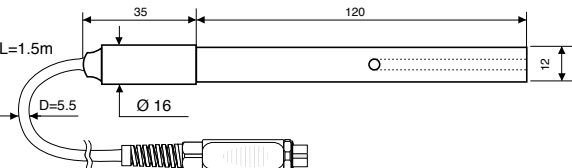ORDERING CODE	MEASUREMENT RANGE AND USE	DIMENSIONS
SP06T	K=0.7 5µS/cm ... 200mS/cm 0...90°C 4-electrode cell in Pocan/Platinum Probe material Pocan General use No heavy tasks	
SPT401.001	K=0.01 0.04µS/cm ... 20µS/cm 0...120°C 2-electrode cell in AISI 316 Ultrapure water Measurement in closed-cell	
SPT01G	K=0.1 0.1µS/cm ... 500µS/cm 0...80°C 2-electrode cell in Platinum-wire Probe material glass Pure water	

2-ring or 4-ring conductivity probes without SICRAM module

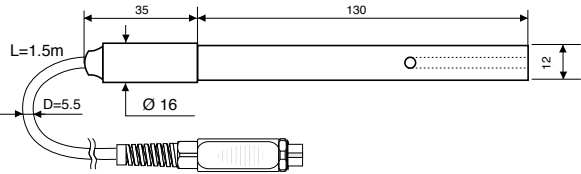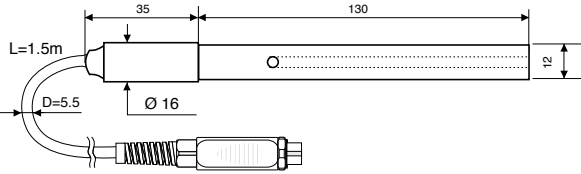ORDERING CODE	MEASUREMENT RANGE AND USE	DIMENSIONS
SPT1G	K=1 10µS/cm ...10mS/cm 0...80°C 2-electrode cell in Platinum wire Probe material glass General heavy tasks, average conductivity	
SPT10G	K=10 500µS/cm ...200mS/cm 0...80°C 2-electrode cell in Platinum wire Probe material glass General heavy tasks, high conductivity	



Conductivity probes with SICRAM module

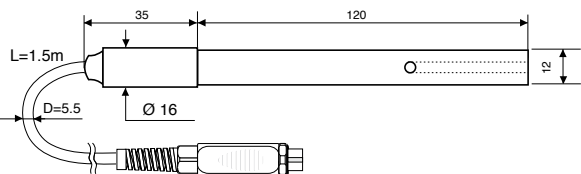ORDERING CODE	MEASUREMENT RANGE AND USE	DIMENSIONS
SPT1GS	K=1 10µS/cm ...10mS/cm 0...80°C 2-electrode cell Glass/Platinum	

Dissolved oxygen probe

Model	D09709 SS	D09709 SS.5
Type	Polarographic probe, Silver anode, Platinum cathode	
Application range		
Application range	0.00...60.00mg/l	
Working temperature	0...45°C	
Accuracy	±1%f.s.	
Membrane	Replaceable	
Cable length	2m	5m (*)

(*)Cable with connector

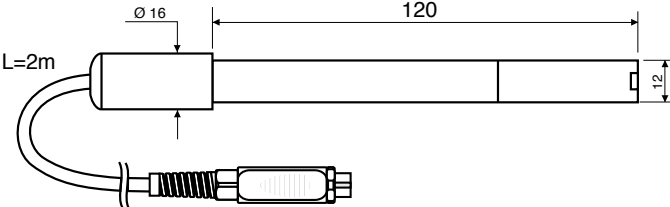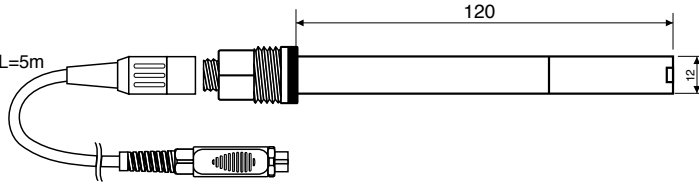D09709SS	
D09709SS.5	

Temperature probes

Pt100 temperature probes with SICRAM module

Modell	Type	Application range	Accuracy
TP87	Immersion	-50°C...+200°C	±0.25°C (-50°C...+200°C)
TP4721.0	Immersion	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP473P.0	Penetration	-50°C...+400°C	±0.25°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP474C.0	Contact	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP475A.0	Air	-50°C...+250°C	±0.3°C (-50°C...+250°C)
TP4721.5	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)
TP4721.10	Immersion	-50°C...+400°C	±0.3°C (-50°C...+350°C) ±0.4°C (+350°C...+400°C)

Temperature drift @20°C 0.003%/°C

4 wires Pt100 probes or 2 wires Pt1000 probes equipped with TP47 module

Modell	Type	Application range	Accuracy
TP47.100	Pt100 4 wires	-50...+200°C	Class A
TP47.1000	Pt1000 2 wires	-50...+200°C	Class A
TP87.100	Pt100 4 wires	-50...+200°C	Class A
TP87.1000	Pt1000 2 wires	-50...+200°C	Class A

Temperature drift @20°C 0.005%/°C

TP47: Module for the connection of Pt100 4-wire and Pt1000 2-wire probes.



HD 22.2
HD 22.3



HD 22.2 - HD 22.3 ELECTRODE HOLDER

HD 22.2: Laboratory electrode holder composed of base plate with built-in magnetic stirrer, shaft and replaceable electrode holder. Suitable diameter 12mm. Powered by bench top instruments of the series **HD22...** with cable **HD22.2.1** (optional), or with power supplier **SWD10** (optional).

HD 22.3: Laboratory electrode holder with base plate. Flexible arm for free positioning. Suitable for electrodes with diameter 12mm.



HD22.2

HD22.3



HD 40.1, HD 40.2 PORTABLE THERMAL PRINTER

The **HD40.1** and **HD40.2** are lightweight, compact, portable thermal printers.

The **HD40.1** is connected to instruments or PC through the **RS232** serial input.

The **HD40.2** features a dual mode data reception system - **RS232** serial and **Bluetooth**. The Bluetooth wireless connection makes the HD40.2 printer very useful "in the field", since it does not require any connection to the instrument. A careful design allows you to replace the thermal paper roll in a few seconds. A four **NiMH rechargeable** battery pack provides power supply and ensures long autonomy: you can print up to 3000 lines at full charge.

Standard thermal paper roll width: 57mm.

Print resolution: 203 dpi

Print characters (each line): 24

Protection degree: IP40.

SPECIFICATIONS

Printing method	Thermal
Resolution	203 DPI (8 dot/mm)
Printing width	48mm centered in the paper roll
Paper roll width	57mm ... 58mm
Max. paper roll diameter	32mm
Number of columns	24
Printing speed	Up to 90 mm/sec (depending on battery charge and ambient conditions)

Sensors	Paper detection
Character set	IBM II 858 table
Printing formats	Normal or extended
Character font	1 (16 x 24 dot – 2mm x 3mm)

Thermal head durability	
Mechanism life	100 million pulses (temperature: 20...25°C)
Abrasion resistance	50km of paper (temperature: 20...25°C)
Cover group durability	2000 opening/closing cycles or more

Communication interfaces	RS232
Bluetooth (for HD40.2)	
RS232 Baud rate	9600, 19200 and 38400 baud (the factory parameter is 38400 baud)
Bluetooth Baud rate	38400 baud (for HD40.2)
Bluetooth operating distance	Up to 10m without hindrance (for HD40.2)
Mains power supply (cod. SWD10)	100-240Vac/12Vdc-1A mains battery charger
Batteries	Four 1.2V AA rechargeable batteries (NiMH)
Printing autonomy	3000 lines 24 characters each. It prints one line every 10 seconds
Switch-off function	0, 5, 10 or 15 minutes
Dimensions	105mm x 165mm x 53mm
Weight	380g (with batteries and paper roll)
Material	ABS

OPERATING CONDITIONS

Operating temperature	0°C ... 50°C
Operating relative humidity	20%RH ... 85%RH not condensing
Storage Temperature / Relative humidity	-25°C ... +70°C / 10%RH ... 90%RH not condensing
Protection degree	IP40

Connections

Serial interface	9-pole D sub male connector
Battery charger power supply (cod. SWD10)	2-pole connector (positive in the middle)

ORDERING CODES

HD40.1: The kit includes: 24-column portable thermal printer, **serial interface RS232**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

HD40.2: The kit includes: 24-column portable thermal printer, **Bluetooth and serial interface RS232**, 57mm paper width, four NiMH 1.2V rechargeable batteries, SWD10 power supply, instruction manual, 5 thermal paper rolls.

The serial cable for PC/instrument connection must be ordered separately.

HD2110CSNM: RS232C 8-pole MiniDin - 9-pole D Sub female null-modem cable for connecting the printer to instruments with MiniDIN connector (HD21xx.1 and HD21xx.2 series, HD34xx.2, HD2010, HD2110, etc.).

9CPRS232: RS232C 9-pole D Sub female null-modem cable for connecting the printer to instrument with 9-pole D Sub connectors (Delta Ohm instruments: HD22xx.2 series, HD98569, HD25.2, etc.).

SWD10: 100-240Vac/12Vdc-1A Mains battery charger.

BAT.40: Spare battery pack for HD40.1 and HD40.2 printers with in-built temperature sensor.

RCT: The kit includes 4 thermal paper rolls 57mm wide and 32mm diameter.





HD 25.2 BENCH-TOP TURBIDITY METER

The **HD25.2** is a digital turbidity meter for laboratory and mobile use, suitable for measurements in drinking water, waste water and process liquids. The working principle is based on the nephelometric (90° scattered light sensor) method.

It is equipped with three light detectors and two LED light sources (white and infrared) which are permanently kept under control in order to guarantee long-term stability. The instrument performs measurements according to the standards **EPA 180.1, ISO-NEPH (ISO 7027), EBC and ASBC**. It is also able to carry out measures of transmission factor percentage of white and infrared light.

The initial factory calibration is based on Forazin primary standard. For routine calibration a set of stabilized secondary standard solutions is available: STCAL (Turbidity standards for calibration):

- **STCAL 1** less than 0,05 NTU
- **STCAL 2** equal to 8 NTU
- **STCAL 3** equal to 80 NTU
- **STCAL 4** equal to 800 NTU



User Calibration is automatic on one, three or four points, depending on the measuring variable.

Stabilized power supply and advanced electronics guarantee optimal performances over time.

The HD25.2 is a **datalogger** that stores up to 999 samples.

The data can be transferred from the instrument connected to a PC via the multi-standard RS232C serial port and USB 2.0.

The RS232C serial port can be used to transfer the acquired measurements to a 24 column printer.

The Print function allows to print labels with progressive numeration and automatic incrementation, with all data related to the sample being examined.

The dedicated software **DeltaLog11** allows instrument management and data processing on PC.

The use of the HD25.2 by more customers is facilitated by the "User Management" function, which allows, according to the case, to enable or disable some advanced functions of the instrument through password.

The protection degree is IP66.

Technical characteristics

Instrument

Dimensions (Length x Width x Height)	220x120x55mm
Weight	400g (batteries included)
Materials	ABS
Display LCD	4½ characters plus symbols Visible area: 52x42mm

Operating conditions

Instrument working temperature	0 ... 50°C
Storage temperature instrument	-25 ... 65°C
Working relative humidity	0 ... 90% R.H. without condensation
Storing of Calibration standards	5...25°C (temperature should not exceed, protect from light)

Protection degree

IP66

Power supply

Batteries	3 1,5 V AA type batteries
Autonomy	100 hours with 1800mAh alkaline
Rete (cod. SWD10)	Mains adapter 100-240Vac/12Vdc-1A

Measuring methods

Standard	EPA180.1, ISO-NEPH (ISO 7027), EBC, ASBC, WHITE %T e IR %T
Light source	LED IR (850nm) and white LED (470nm)
Receiver	Silicium photodiode
Sample cell	Ø24mm - height 68mm, 20cc



Measurement of turbidity

Method / Measuring range

EPA180.1	(0...1000 NTU)
ISO-NEPH	(0...1000 FNU)
EBC	(0...250 EBC)
ASBC	(0...9999 ASBC)
WHITE %T	(0...100 %T)
IR %T	(0...100 %T)
Resolution	0.01 NTU (0...9.99 NTU)
	0.1 NTU (10.0...99.9 NTU)
	1 NTU (100...1000 NTU)
Accuracy	±2% reading + 0.01 NTU (0...500 NTU)
	±3% reading (500...1000 NTU)
Repeatability	±2% reading or 0.01 NTU (the major one)

Security of memorized data

Unlimited

Time

Date and hour

real time schedule

Accuracy

1min/month max error

Measured values storing

Quantity

999 samples

Serial interface RS232C

Type

RS232C electrically isolated

Baud rate

Can be set from 1200 to 38400 baud

Data bit

8

Parity

None

Stop bit

1

Flow Control

Xon/Xoff

Serial cable length

Max 15m

USB interface

Type

1.1 - 2.0 electrically isolated

Connections

Serial interface

DB9 connector (9- pole male)

USB interface

USB connector type B

Mains adapter

2- pole connector (Ø5.5mm-2.1mm). Positive at centre.

Ordering codes

HD25.2K: The kit is composed of: instrument HD25.2, 4 empty cells, 4 calibration standards STCAL, 3 1.5Vdc alkaline batteries, lubricant rag, 25cc Silicon oil, instructions manual, carrying case and software DeltaLog11 for PCs running Windows 98 to Vista.

Accessories

9CPRS232: Connection cable SubD female 9- pole for serial output RS232C

CP22: Connection cable USB 2.0 connector type A - type B

SWD10: Stabilized power supply at 230Vac/9Vdc-300mA mains voltage.

HD40.1: Portable, serial input, 24 column thermal printer, 57mm paper width.

PL: Lubricant rag

OS1: Silicon oil - 25cc.

KCV: 4 empty sample cells Ø24x68mm

Turbidity calibration standards

STCAL 1: Calibration standard with low turbidity formazin reference less than 0,05 NTU.

STCAL 2: Calibration standard with reference formazin 8 NTU - 20cc.

STCAL 3: Calibration standard with reference formazin 80 NTU - 20cc.

STCAL 4: Calibration standard with reference formazin 800 NTU - 20cc.

KS: Kit 4 calibration standard with reference formazin STCAL 1, STCAL 2, STCAL 3, STCAL 4.



HD40.1



ASBC



FNU



EBC



NTU

